

HIOSSEN SURGICAL KITS

PRODUCT CATALOG



HIOSSEN
IMPLANT



Hiossen Surgical Kit

Version: PC24HISLTR1.1

270 Sylvan Ave. Ste 1130, Englewood Cliffs, NJ 07632

www.hiossen.com Email: marketing@hiossen.com

@ @hiossen_implants  @HiossenImplants  @Hiossen



Hiossen Surgical Kits

Intro

About us	004
History	005

GUIDED SURGERY KITS

OneGuide Kit	006
OneCAS Kit	016
OneMS Kit	018

IMPLANT KITS

122 Taper Kit	022
Taper Kit & Taper Ultra Kit	030
485 Kit	040
Assist Kit	044
Ultra Kit	046
Denture 4U Kit	058

PROSTHETIC & MAINTENANCE KITS

Prosthetic Simple Kit & Prosthetic Kit	062
EIR Kit & EIR Full Kit	070
ESR Kit & ESR Full Kit	074
IM-Cure Kit	080

SINUS SURGERY KITS

CAS Kit	084
LAS Kit	088

NARROW RIDGE SURGERY KITS

ESSET Kit	090
EM(MS) Kit	094

INSTRUMENTS KIT

Surgical Instruments Kit	098
--------------------------	-----

Legacy Based on Technology


All Hiossen implants are domestically produced, manufactured and packaged in Pennsylvania, USA. Our global production has collaborated with the international distribution network to build a strict quality management system, which includes comprehensive inspection, quality tracking, in house surface treatment and sterilization process.

Hiossen has acquired strict quality certifications such as FDA and CE. Hiossen exports implants worldwide to over 40 countries and its recognized for its technology and quality in the global markets.

With an endless challenge of providing the latest technology, Hiossen is making its way to become one of the top global implant, restorative and digital dentistry companies. Our reliable, convenient and simpler solutions are built on infinite queries, persistence and confidence.

Together with our parent company, Osstem Implant, we became one of the top five dental implant leaders with a far-ranging spectrum of products and services.

Hiossen shares a passion for better life by sophisticating and developing new products and assisting the medical treatment procedures by making them safer and simpler for clinicians and patients. Our team strives to provide the best surgical and restorative outcomes by conducting rigorous testing, research, clinical studies and services, which we have proven through our dedication to improving the quality of life of edentulous patients.

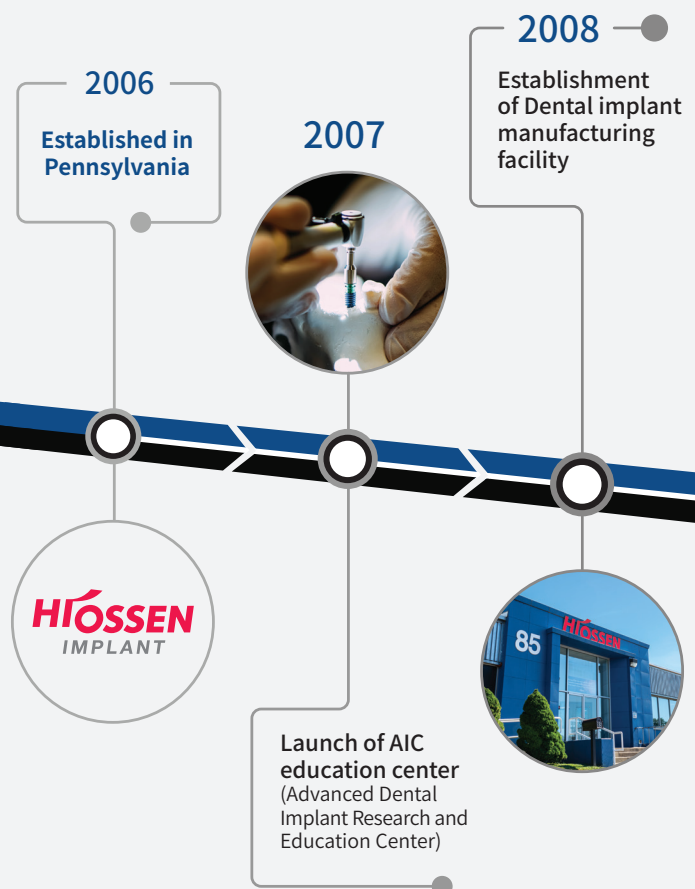



2011



Launch of
ET III SA implant
(Sand-blasted
& Acid-etched)

2013

Establishment
of SmartFit
Center East
(Comprehensive
digital implant
scan, design, milling)

2016



Launch of
ET III NH implant
(Nano-Hydrophilic)

2018

Recognized as
TOP 5 in global
dental implant market

Launched
K3 Unit Chair

2020



Establishment
of SmartFit
Center West

2023

Operating
17 sales regions
& 72 branches
nationwide

Exporting
worldwide to over
70 countries

Launch of
T2 CBCT Scan



The President's
“E” Award

Recognizing Excellence in Exporting



OneGuide Kit (HOGK)

※ OneGuide (EK) Kit: HKOGK

For

EKIII

ETIII/IV


SSII/III

Top panel components


Torque Wrench
TQWCB





Depth Gauge
ODG

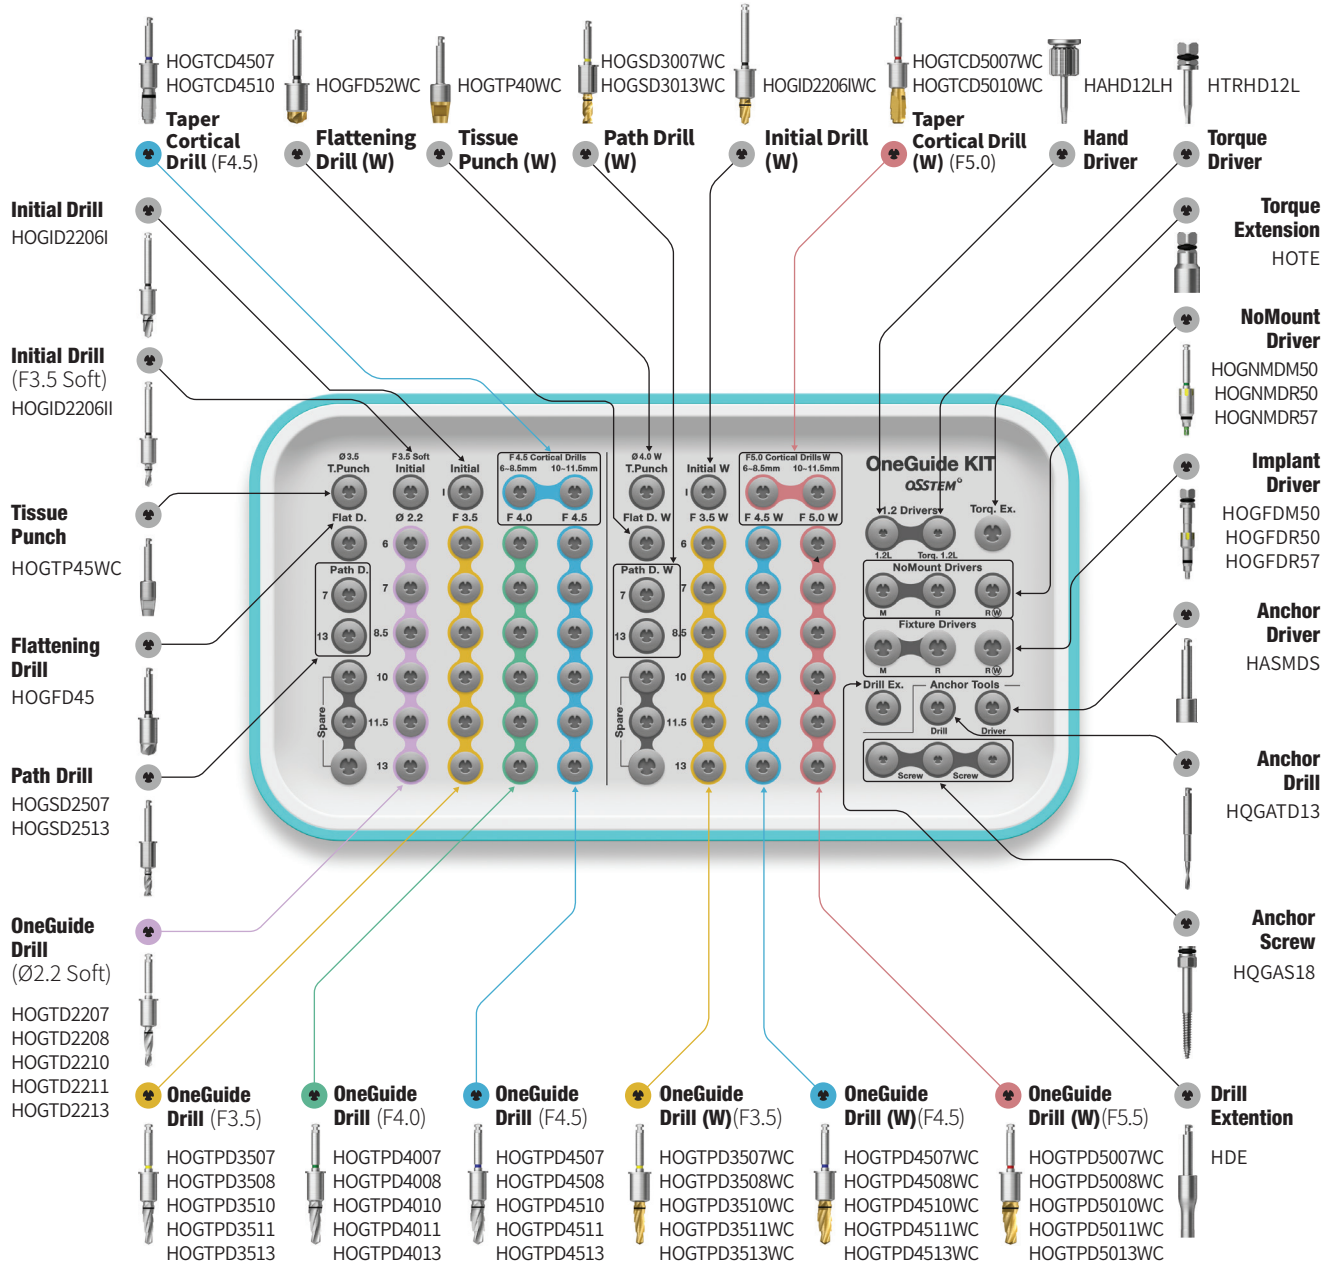



OneGuide Kit Surgical Kit Instruments

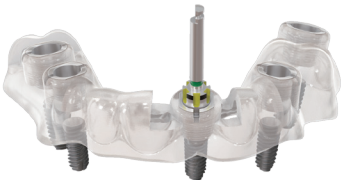OneGuide Template	
Description	Image
<ul style="list-style-type: none"> Two sizes of guide holes depending on the diameter of the implant <ul style="list-style-type: none"> - D5.0 for implant diameters: F3.5/4.0/4.5 - D5.8 for implant diameter: F5.0 Dual contact feature ensures excellent accuracy in positioning and stability Simple drilling sequence by adopting 122 Taper Kit concepts Packing unit: surgical guide (optional: SmartFit abutment, Temporary Crown) 	



Tissue Punch				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used to remove gingiva flaplessly 7 types according to the OneGuide guide holes Drills except two types are not included in the Kit (HOGTP35R, HOGTP40WC) and are sold separately Recommended speed: 800 ~ 1,200 rpm 	Ø3.0	HOGTP30R	-	
	Ø3.5	HOGTP35R	-	
	Ø4.0	HOGTP40R	HOGTP40WC	
	Ø4.5	HOGTP45R	HOGTP45WC	
	Ø5.0	-	HOGTP50WC	


Flattening Drill				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used for flattening narrow or irregular bone ridges, before initial drill Multiple cutting edge designed to prevent drill bouncing 2 Types (Below F5.0/for F5.0) Recommended speed: 800 ~ 1,200 rpm 	Ø4.5	HOGFD45	-	
	Ø5.2	-	HOGFD52WC	

Initial Drill				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used after Tissue Punch for initial drilling Secures depth for subsequent drills for more stability Available in 3 types: (F3.5 soft bone/below F5.0/for 5.0) Recommended speed: 800 ~ 1,200 rpm 	Ø3.5 (Soft)	HOGID2206II	-	
	Ø4.0/Ø4.5	HOGID2206I	-	
	Ø5.0 (W)	-	HOGID2206IWC	


Initial Drill (Short Type)				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Short type Initial Drill (5.3mm shorter) Used for limited intermaxillary space Available in 3 types: (F3.5 soft bone/below F5.0/for 5.0) Recommended speed: 800 ~ 1,200 rpm 	Ø3.5 (Soft)	HOGD2206IIS	-	
	Ø4.0/Ø4.5	HOGD2206IS	-	
	Ø5.0 (W)	-	HOGD2206ISWC	


OneGuide Kit Surgical Kit Instruments


OneGuide Drill							
Description/Item code							
<ul style="list-style-type: none">• Taper Drill optimized for III/IV type implant• Used for placing F3.5 ~ F5.0 & 6 ~ 13mm implants• Multi-step drill design allows for stable drilling• Drills for 6mm and F5.5(W) types are sold separately• Recommended speed: Soft Bone (800 ~ 1,200 rpm) / Normal, Hard Bone (1,200 ~ 1,500 rpm)							
Below F5.0 Regular Hole (Ø5.1)		D/Ø	Ø3.5	Ø4.0	Ø4.5	Image/Guide 	
		Y-Dim.	0.7	0.9	1.0		
L	TL	GD	5.0	5.0	5.0		
6	36.1		HOGTPD3506	HOGTPD4006	HOGTPD4506		
7	36.1		HOGTPD3507	HOGTPD4007	HOGTPD4507		
8.5	36.1		HOGTPD3508	HOGTPD4008	HOGTPD4508		
10	36.1		HOGTPD3510	HOGTPD4010	HOGTPD4510		
11.5	37.6		HOGTPD3511	HOGTPD4011	HOGTPD4511		
13	39.1		HOGTPD3513	HOGTPD4013	HOGTPD4513		
Below F5.0 Wide Hole (Ø5.8)		D/Ø	Ø3.5 (w)	Ø4.5 (w)	Ø5.0 (w)	Ø5.5 (w)	Image/Guide 
		Y-Dim.	0.7	0.9	1.0	1.0	
L	TL	GD	5.7	5.7	5.7	5.7	
6	36.1		HOGTPD3506WC	HOGTPD4506WC	HOGTPD5006WC	HOGTPD5506WC	
7	36.1		HOGTPD3507WC	HOGTPD4507WC	HOGTPD5007WC	HOGTPD5507WC	
8.5	36.1		HOGTPD3508WC	HOGTPD4508WC	HOGTPD5008WC	HOGTPD5508WC	
10	36.1		HOGTPD3510WC	HOGTPD4510WC	HOGTPD5010WC	HOGTPD5510WC	
11.5	37.6		HOGTPD3511WC	HOGTPD4511WC	HOGTPD5011WC	HOGTPD5511WC	
13	39.1		HOGTPD3513WC	HOGTPD4513WC	HOGTPD5013WC	HOGTPD5513WC	


Twist Drill						
Description		F3.5 Soft Bone Regular Hole (Ø5.1)		D/Ø	Ø2.2	Image/Guide
				Y-Dim.	0.7	
		L	TL	GD	5.0	
<ul style="list-style-type: none">• Used to place F3.5 implants in soft bone• Available in 5 types• Recommended speed: 800 ~ 1,200 rpm		7	36.1		HOGTD2207	
		8.5	36.1		HOGTD2208	
		10	36.1		HOGTD2210	
		11.5	37.6		HOGTD2211	
		13	39.1		HOGTD2213	

OneGuide Kit Surgical Kit Instruments

OneGuide Vertical Twist Drill				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used for drilling before OneGuide Anchor Sold as an individual item Recommended speed: 800 ~1,200 rpm 	Ø1.5	HOGTD1506	HOGTD1506W	

OneGuide Vertical Bone Anchor				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used for fixing the OneGuide in place (e. g. edentulous case) Mounted on the alveolar bone vertically to fix OneGuide in place Soft bone: placed directly Normal/hard bone: placed after using the OneGuide Vertical Drill Tighten at 20 rpm with Anchor Driver Sold as an individual item 	Ø2.0	HOGBAR	HOGBAW	

OneGuide Vertical Implant Anchor				
Description	D/Ø	Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Used for fixing OneGuide in place (e. g. edentulous case) Mounted on the implant vertically to fix OneGuide in place Tighten with 1.2 hex Hand Driver Only used for Regular connection of F4.0 or greater Sold as an individual item 	Ø2.0	HOGFAR	HOGFAW	

OneGuide NoMount Driver for ET				
Description	*C	D/Ø	Item code	Image/Guide
<ul style="list-style-type: none"> Used to place a NoMount implant It is recommended to place the implant ~80% of the planned implant depth with this driver *C = Connection 	F3.5	Mini Regular Hole (Ø5.1)	HOGNMDM50	
	F4.0/4.5	Regular Regular Hole (Ø5.1)	HOGNMDR50	
	F5.0	Regular Wide Hole (Ø5.8)	HOGNMDR57	




OneGuide Kit Surgical Kit Instruments




OneGuide Implant Driver for ET				
Description	*C	D/Ø	Item code	Image/Guide
<ul style="list-style-type: none"> Used with a wrench for finishing the final implant placement Yellow groove aligns the abutment hex direction Match the grooves on the OneGuide template with the grooves on the driver *C = Connection 	F3.5	Mini Regular Hole (Ø5.1)	HOGFDM50	
	F4.0/4.5	Regular Regular Hole (Ø5.1)	HOGFDR50	
	F5.0 (W)	Regular Wide Hole (Ø5.8)	HOGFDR57	




Implant Driver (Stopper Type)				
Description	*C	D/Ø	Item code	Image/Guide
<ul style="list-style-type: none"> Featuring stopper design to prevent entry below the upper surface of OneGuide hole Sold as an individual item *C = Connection 	F3.5	Mini Regular Hole (Ø5.1)	HOGFDSM50	
	F4.0/4.5	Regular Regular Hole (Ø5.1)	HOGFDSR50	
	F5.0 (W)	Regular Wide Hole (Ø5.8)	HOGFDSR57	




OneGuide Taper Cortical Drill			
Description	L	Regular Hole (Ø5.1)	Image/Guide
<ul style="list-style-type: none"> Used for placing F4.5 and F5.0 implants in hard bone Optimize placement by cutting cortical bone Drills for 13 mm diameter implant is sold separately Drilling up to the first black line for 6mm placement Recommended speed: 800 ~ 1,200 rpm 	6 / 7 / 8.5mm 10 / 11.5mm 13mm	HOGTCD4507 HOGTCD4510 HOGTCD4513	
	L	Wide Hole (Ø5.8)	

OneGuide Kit Surgical Kit Instruments



OneGuide No Mount Driver for EK				
Description	*C	D/Ø	Item code	Image/Guide
<ul style="list-style-type: none"> Used for placing EK NoMount Implants Recommended to place ~80% of the planned implant depth with this driver Sold as an individual item *C = Connection 	F3.5	Regular Regular Hole (Ø5.1)	HOGNMDM50K	
	F4.0/4.5		HOGNMDR50K	
	F5.0	Regular Wide Hole (Ø5.8)	HOGNMDR57K	


OneGuide Implant Driver for EK				
Description	*C	D/Ø	Item code	Image/Guide
<ul style="list-style-type: none"> Used with a wrench for finishing the final implant placement Yellow groove aligns the abutment hex direction Match the grooves on the OneGuide template with the grooves on the driver Sold as an individual item *C = Connection 	F3.5	Regular Regular Hole (Ø5.1)	HOGFDM50K	
	F4.0/4.5		HOGFDR50K	
	F5.0	Regular Wide Hole (Ø5.8)	HOGFDR57K	

OneGuide NoMount Driver for SS				
Description	*P	D/Ø	Item code	Image
<ul style="list-style-type: none"> Used for placing SS NoMount Implants Recommended to place ~80% of the planned implant depth with this driver *P = Platform 	F3.5/F4.0/4.5	Mini Regular Hole (Ø5.1)	HOGNMDR50S	
	F5.0	Regular Wide Hole (Ø5.8)	HOGNMDR57S	
	F5.0	Wide Extra Wide Hole (Ø6.8)	HOGNMDW67S	


OneGuide Implant Driver for SS				
Description	*P	D/Ø	Item code	Image
<ul style="list-style-type: none"> Used with a wrench for finishing the final implant placement Yellow groove aligns the abutment hex direction Match the grooves on the OneGuide template with the grooves on the driver Sold as an individual item *P = Platform 	F3.5/F4.0/4.5	Mini Regular Hole (Ø5.1)	HOGFDR50S	
	F5.0	Regular Wide Hole (Ø5.8)	HOGFDR57S	
	F5.0	Wide Extra Wide Hole (Ø6.8)	HOGFDW67S	

OneGuide Kit Surgical Kit Instruments

OneGuide Path Drill					
Description	L		Regular Hole (Ø5.1)	Wide Hole (Ø5.8)	Image/Guide
<ul style="list-style-type: none"> Drill for correcting path deviation during OneGuide surgery Used for creating implant placement path for extraction cases Flat blade design optimized for cutting inclined bone 4 types for each OneGuide hole diameter, 8 types in total: Regular hole (Ø5.1) / Wide hole (Ø5.8) For 13mm drills, depth is adjusted according to the black lines Recommended speed: 1.200 ~ 1,500 rpm 	7	Ø2.5	HOGSD2507	HOGSD2507WC	
		Ø3.0	HOGSD3007	HOGSD3007WC	
	13	Ø2.5	HOGSD2513	HOGSD2513WC	
		Ø3.0	HOGSD3013	HOGSD3013WC	

Anchor Screw		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to affix the OneGuide firmly Selectable at the preoperative planning stage 	HQGAS18	

Anchor Drill		
Description	Item Code	Image
<ul style="list-style-type: none"> Used for drilling before using anchor screw Recommended speed: 800 ~ 1.200 rpm 	HQGATD13	


OneGuide Anchor Driver (Mount Driver)		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to place anchor screw 	HASMDS	

Drilling Sequence **OneGuide Drill**


EKIII | ETIII

(Length: 10mm)


Ø3.5

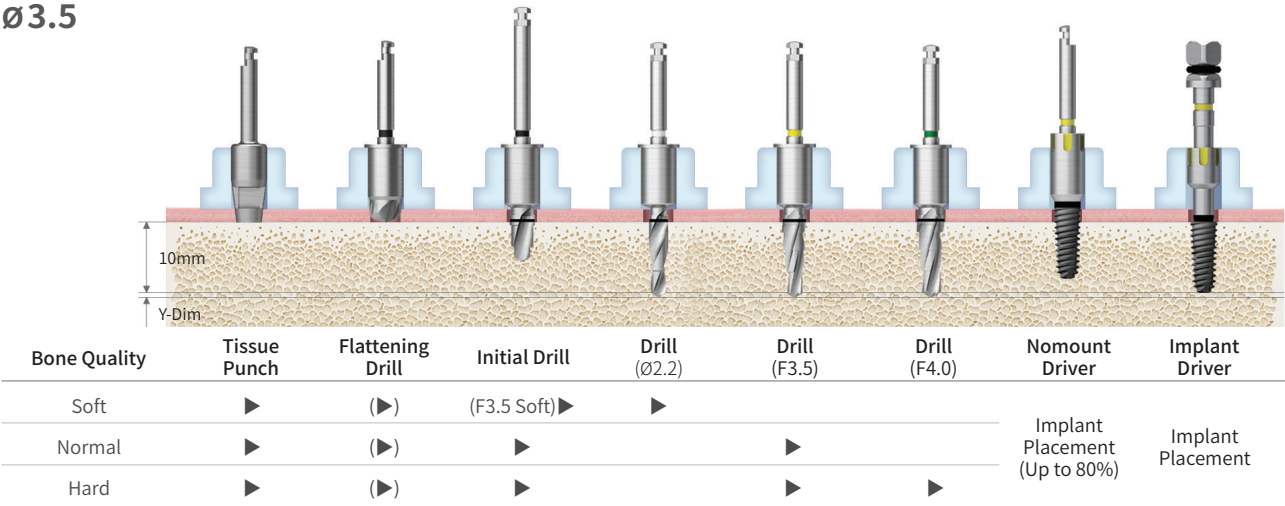

Ø4.0

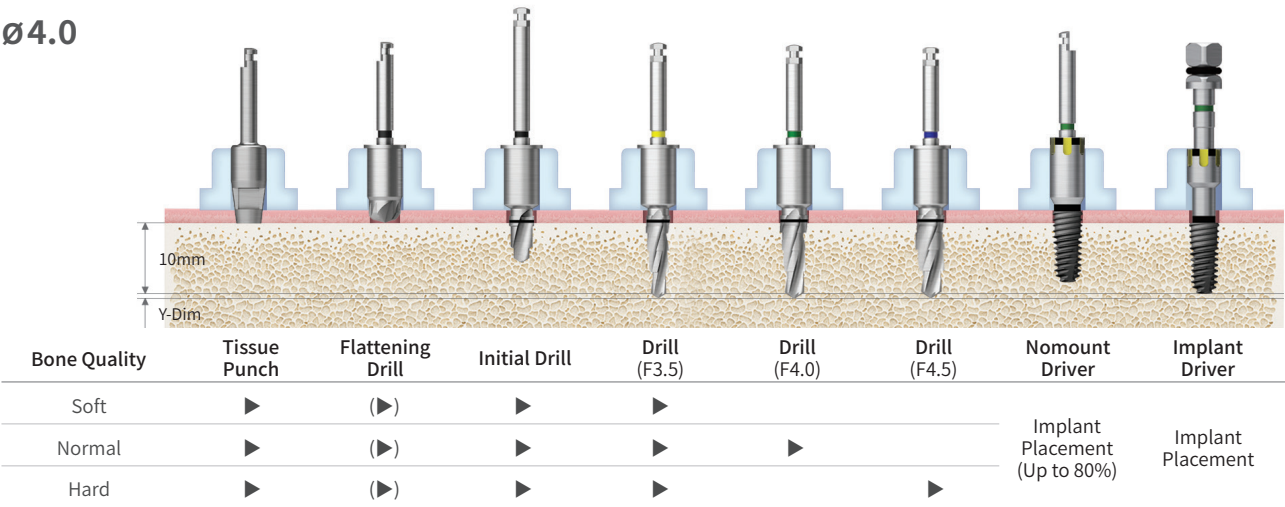

Ø4.5

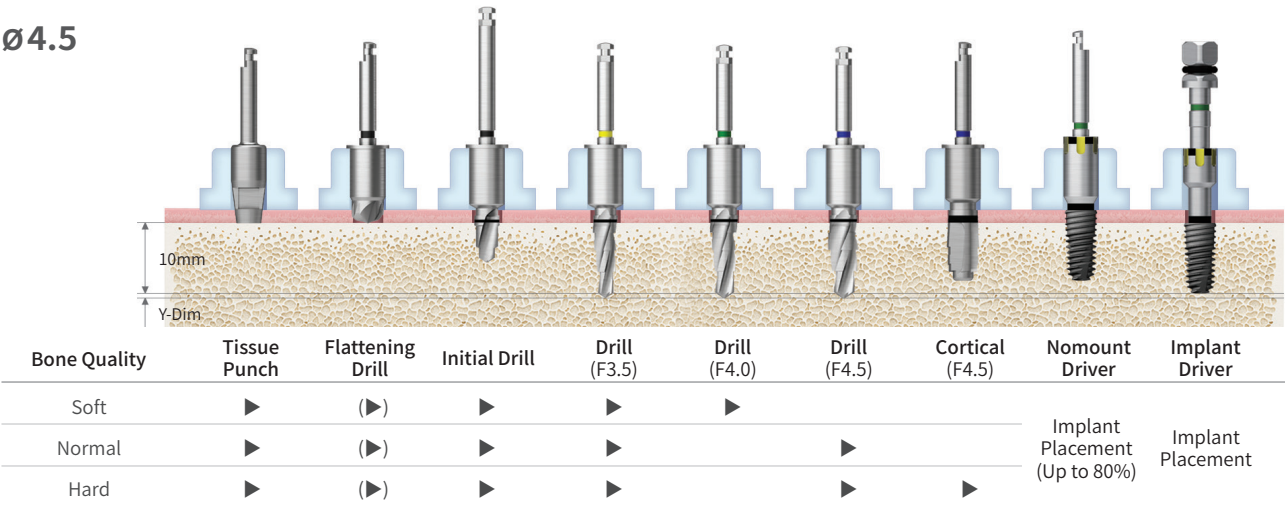


Drilling Sequence OneGuide Drill

EKIII | ETIII

(Length: 10mm)


Ø5.0

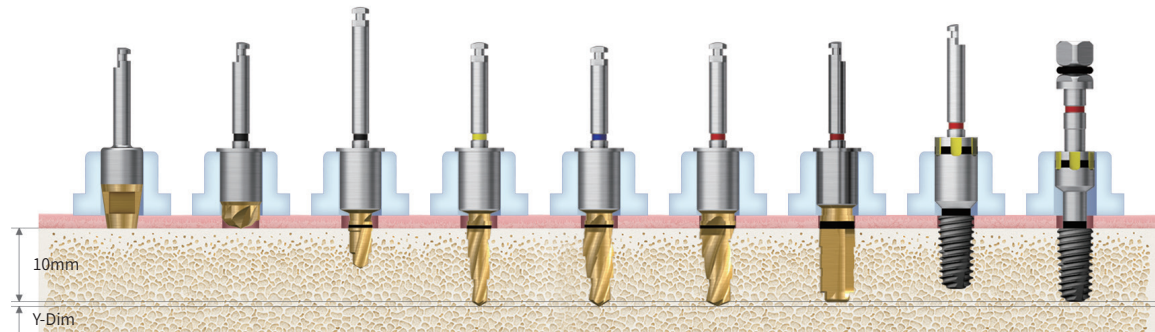

Bone Quality	Tissue Punch (W)	Flattening Drill (W)	Initial Drill (W)	Drill (W) (F3.5)	Drill (W) (F4.5)	Drill (W) (F5.0)	Cortical (W) (F5.0)	Nomount Driver	Implant Driver
Soft	►	(►)	►	►	►				
Normal	►	(►)	►	►		►		Implant Placement (Up to 80%)	Implant Placement
Hard	►	(►)	►	►		►	►		


※ For extra short implants (Ø4.0, Ø4.5 / 6mm) only

Ø4.0

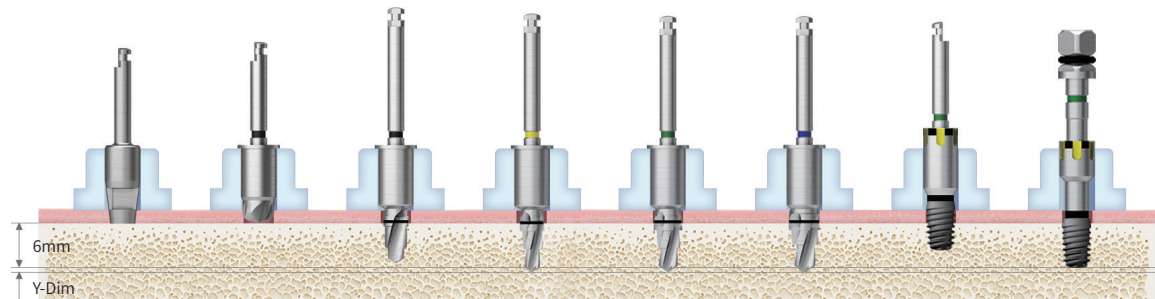

Bone Quality	Tissue Punch	Flattening Drill	Initial Drill	Drill (F3.5)	Drill (F4.0)	Drill (F4.5)	Nomount Driver	Implant Driver
Soft	►	(►)	►	F3.5x6				
Normal	►	(►)	►	F3.5x6	F4.0x6		Implant Placement (Up to 80%)	Implant Placement
Hard	►	(►)	►	F3.5x6		F4.5x6		

Ø4.5

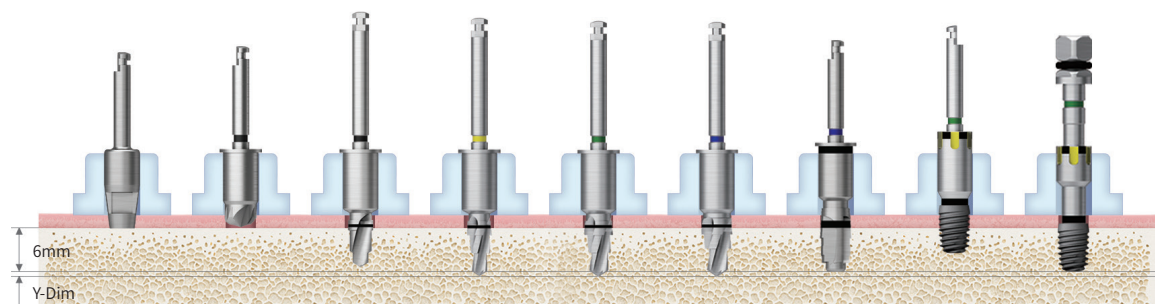


Bone Quality	Tissue Punch	Flattening Drill	Initial Drill	Drill (F3.5)	Drill (F4.0)	Drill (F4.5)	Cortical (F4.5)	Nomount Driver	Implant Driver
Soft	►	(►)	►	F3.5x6	F4.0x6				
Normal	►	(►)	►	F3.5x6		F4.5x6		Implant Placement (Up to 80%)	Implant Placement
Hard	►	(►)	►	F3.5x6		F4.5x6	F4.5x6~8.5		

ETIV


(Length: 10mm)

Ø4.0

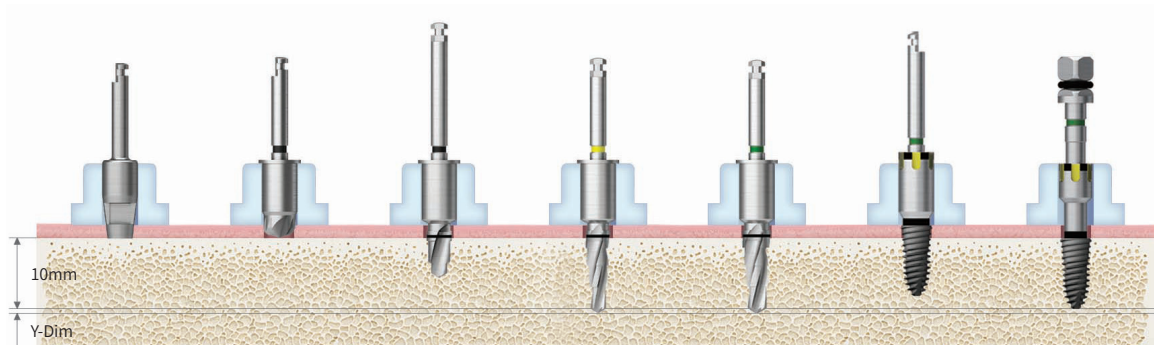


Bone Quality	Tissue Punch	Flattening Drill	Initial Drill	Drill (F3.5)	Drill (F4.0)	Nomount Driver	Implant Driver
Soft	►	(►)	►	►		Implant Placement (Up to 80%)	Implant Placement
Normal	►	(►)	►	►	►		

Ø4.5

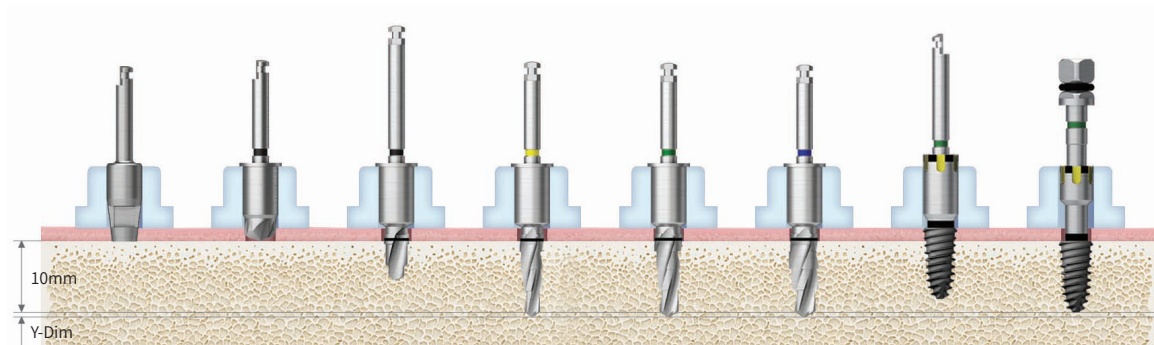

Bone Quality	Tissue Punch	Flattening Drill	Initial Drill	Drill (F3.5)	Drill (F4.0)	Drill (F4.5)	Nomount Driver	Implant Driver
Soft	►	(►)	►	►	►		Implant Placement (Up to 80%)	Implant Placement
Normal	►	(►)	►	►		►		

Ø5.0

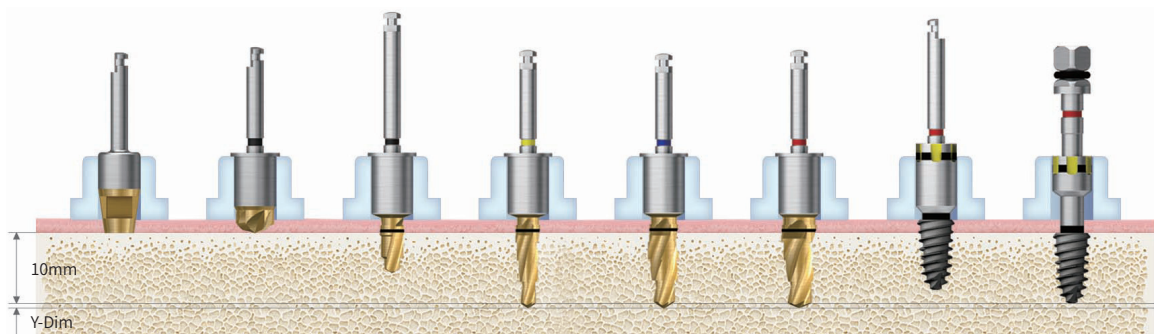

Bone Quality	Tissue Punch (W)	Flattening Drill (W)	Initial Drill (W)	Drill (W) (F3.5)	Drill (W) (F4.5)	Drill (W) (F5.0)	Nomount Driver	Implant Driver
Soft	►	(►)	►	►	►		Implant Placement (Up to 80%)	Implant Placement
Normal	►	(►)	►	►		►		

OneCAS Kit (HOCK)

For

EKIII

ETIII/IV

Hydraulic Membrane Lifter Tube
SNMT



Bone Condenser
SNBC1114



Top panel components

Depth Gauge
HCDG



Depth Gauge(W)
HCDGW




Lower panel components


Bone Carrier Head
SNBCH30






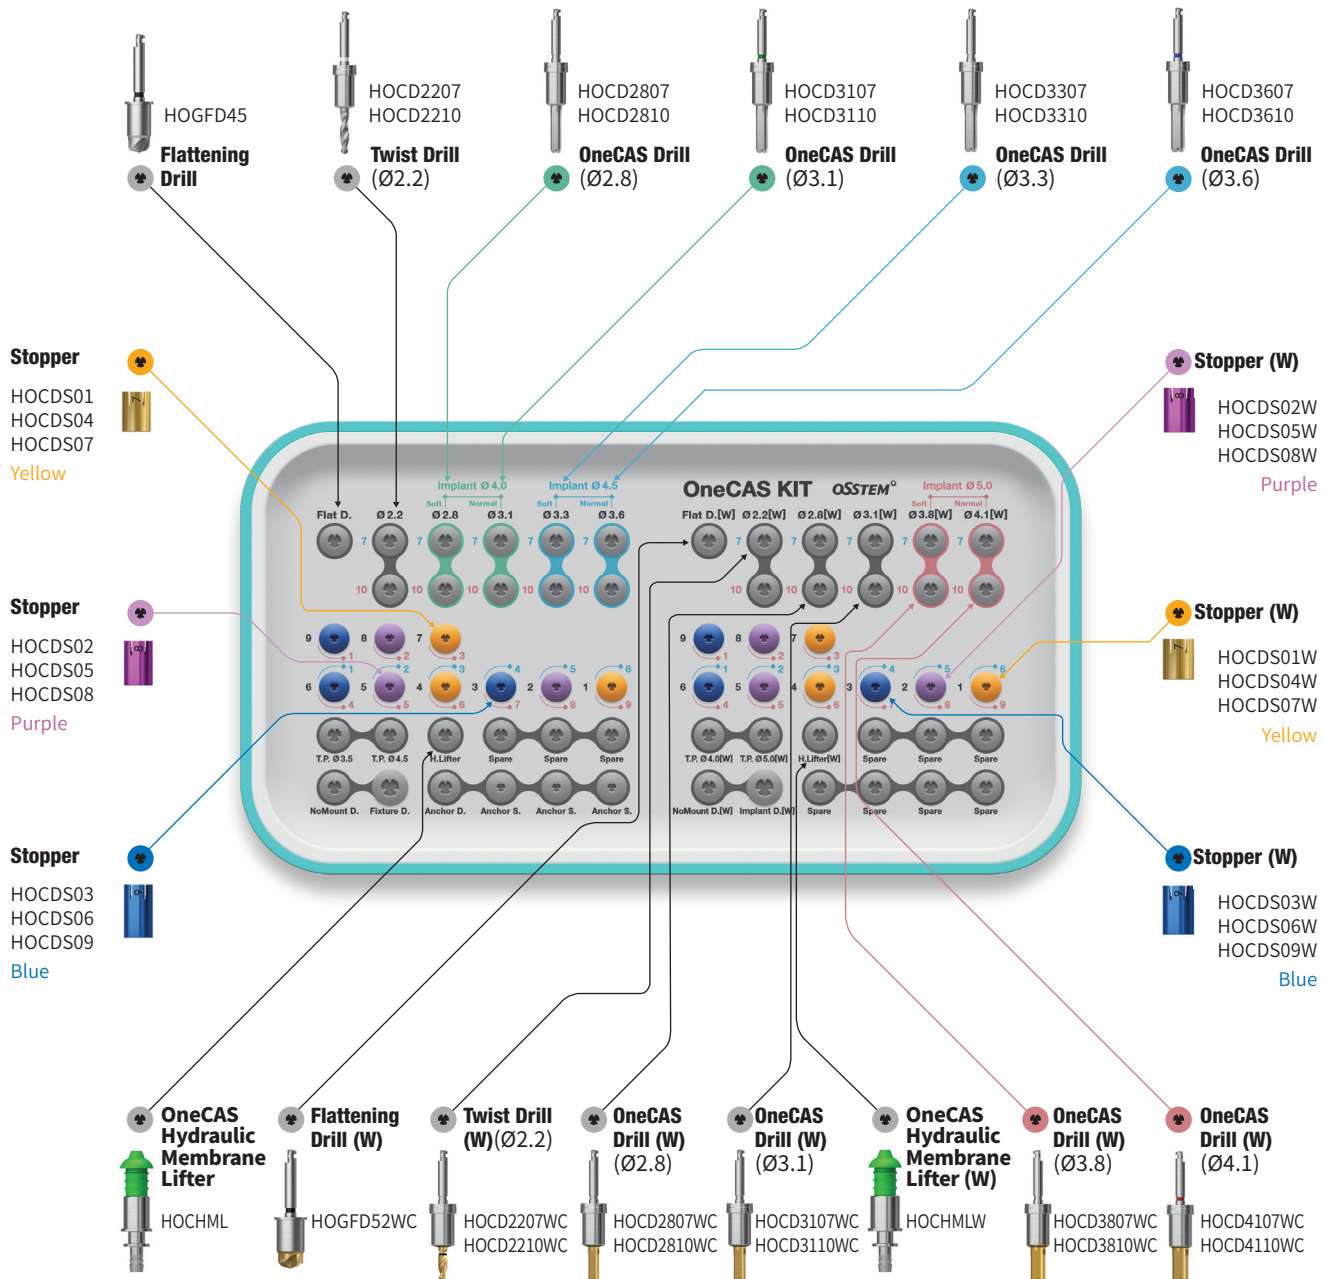



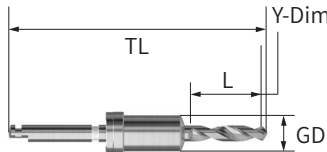


Bone Carrier
SNBCS35




OneCAS Kit Surgical Kit Instruments

OneCAS Twist Drill							
Description				F4.0/4.5	F5.0 (W)	Image/Guide	
<ul style="list-style-type: none">• Recommended to drill 1mm under the lower margin of maxillary sinus• Used with a stopper for a safe membrane approach• 1mm shorter than a normal Twist Drill• Recommended speed: 400 ~ 1,200 rpm	Y-Dim			0.6			
	GD			5.0	5.7		
	TL	L	D/Ø	HOCD2207 HOCD2210	HOCD2207WC HOCD2210WC		
	33.2 36.2	7 10	Ø2.2				

OneCAS Drill							
Description	F4.0/4.5		Ø2.8	Ø3.1	Ø3.3	Ø3.6	Image/Guide
<ul style="list-style-type: none">Used with the stopper of OneCAS systemThe membrane is safely lifted during maxillary sinus surgeryPossible to collect autogenous bone at low RPM'sUse a stopper for a safe membrane approachFinal drill diameter selection based on bone qualityRecommended rpm: 400~800rpm	L	TL	5.0				
	7	33.6	HOCD2807	HOCD3107	HOCD3307	HOCD3607	
	10	36.1	HOCD2810	HOCD3110	HOCD3310	HOCD3610	
	F5.0 (W)		Ø2.8	Ø3.1	Ø3.8	Ø4.1	
	L	TL	5.0				
	7	33.6	HOCD2807WC	HOCD3107WC	HOCD3807WC	HOCD4107WC	
	10	36.6	HOCD2810WC	HOCD3110WC	HOCD3810WC	HOCD4110WC	

OneCAS Stopper									
<ul style="list-style-type: none"> Stopper number indicates the length when engaged On the Kit, protruding length marked in blue for 7mm drills and in red for 10mm drills Color coded by length Recommended number of use: 50 times 									
Diameter	1	2	3	4	5	6	7	8	9
									
F4.0/4.5	HOCDs01	HOCDs02	HOCDs03	HOCDs04	HOCDs05	HOCDs06	HOCDs07	HOCDs08	HOCDs09
F5.0 (W)	HOCDs01W	HOCDs02W	HOCDs03W	HOCDs04W	HOCDs05W	HOCDs06W	HOCDs07W	HOCDs08W	HOCDs09W
Color	Yellow	Purple	Blue	Yellow	Purple	Blue	Yellow	Purple	Blue

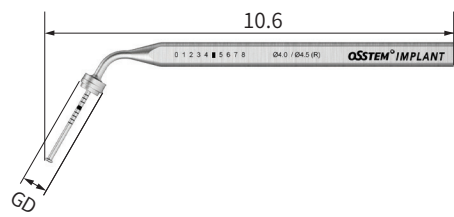Depth Gauge			
Description		F4.0/4.5	F5.0 (W)
	GD	5.0	5.7
<ul style="list-style-type: none"> Checks for internal sinus lift Measures residual bone depth Use with a stopper for safer approach Same depth marking lines as a 10mm drill 	HCDG	HCDGW	

OneMS Kit (HOMSK)

For

EKIII


ETIII/IV

EM(MS)

Top panel components



Torque Wrench

TQWCB





Depth Gauge


HMDTGG

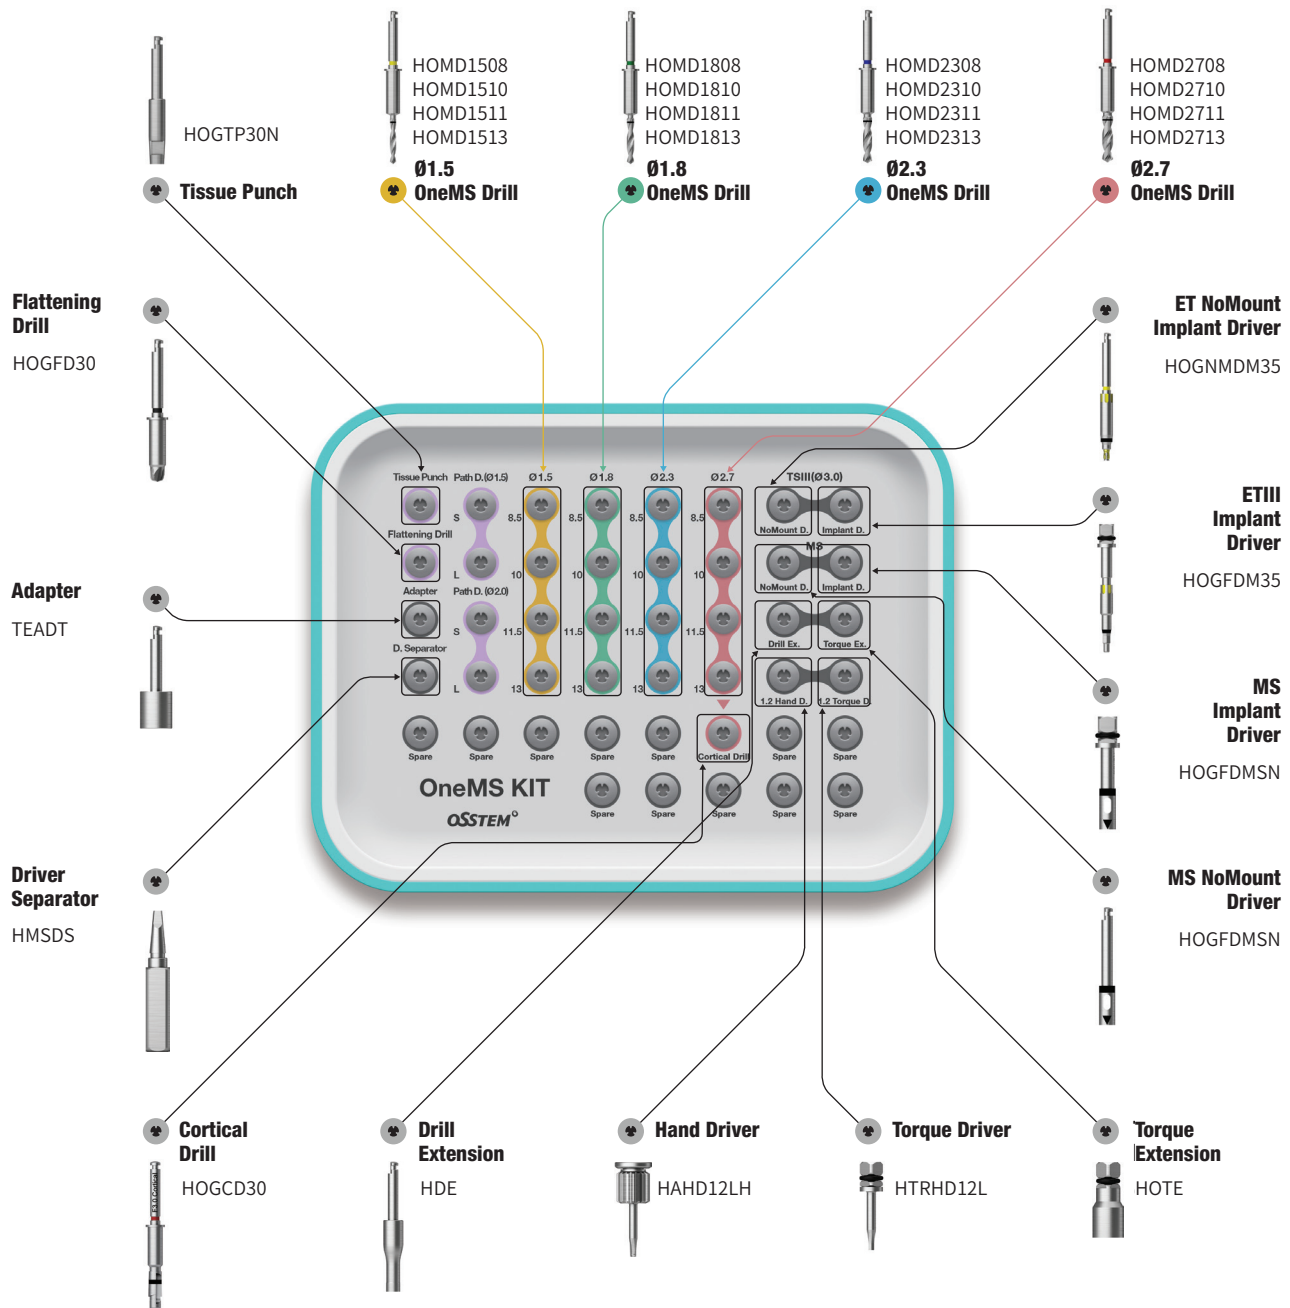

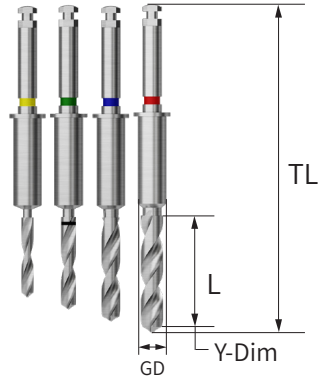

OneMS Kit Surgical Kit Instruments

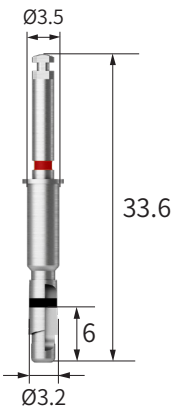OneMS Drill							Image/Guide	
Description/Item code							Image/Guide	
<ul style="list-style-type: none"> Straight type drills for EM implant / ETIII Ø3.2 implants (EM Ø2.0 ~ Ø3.0 / ETIII Ø3.2 implants) OneMS Cortical Drill is used for placing ETIII Ø3.2 implants in hard bones Start with 8.5mm drill for stable drilling Recommended speed: 800 ~ 1,200 rpm 								
L	TL	D/Ø	Ø1.5	Ø1.8	Ø2.3	Ø2.7		
		GD	0.6	0.6	0.6	0.6		
8.5	37.5		HOMD1508	HOMD1808	HOMD2308	HOMD2708		
10	39		HOMD1510	HOMD1810	HOMD2310	HOMD2710		
11.5	40.5		HOMD1511	HOMD1811	HOMD2311	HOMD2711		
13	42		HOMD1513	HOMD1813	HOMD2313	HOMD2713		
Color			Yellow	Green	Blue	Pink		

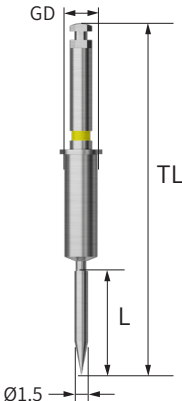
OneMS Cortical Drill	
Description/Item code	Image
<ul style="list-style-type: none"> Used to remove cortical bone in hard bone Used for expanding the cortical bone after using the Straight Drill (ETIII Ø3.0 only) Recommended speed: 800 ~ 1,200 rpm 	
HOGCD30	


OneMS Lance Drill				
Description/Item code			Image/Guide	
<ul style="list-style-type: none">Creates holes in the bone to facilitate initial drillingBone density can be determined through drillingSingle item (excluded from OneMS Kit)				
L	TL	D/Ø		Ø1.5
8.5	37.5			HOMLD1508
10	39			HOMLD1510
11.5	40.5			HOMLD1511
13	42			HOMLD1513


Flattening Drill	
Description/Item code	Image
<ul style="list-style-type: none"> Used for narrow or uneven ridges Cutting edge design allows for stable bone removal 	
HOGFD30	


Driver Separator	
Description/Item code	Image
<ul style="list-style-type: none"> Used in case a driver is wedged with the implant during insertion Insert the Driver Separator into the driver groove to loosen it from the implant 	
HMSDS	


OneMS Kit Surgical Kit Instruments

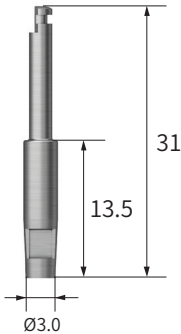Tissue Punch	
Description/Item code	Image
<ul style="list-style-type: none"> Used to remove gingiva to continue with flapless surgery 	
HOGTP30N	

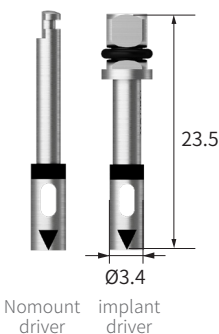OneMS Driver	
Description	Image
<ul style="list-style-type: none"> Used with the torque wrench for adjustment of the final implant placement for MS implant narrow ridge Match the mark with the implant 	
F2.0/2.5/3.0	
HOGFMSN	

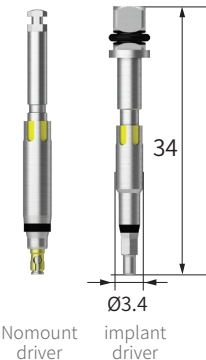ET Implant Driver	
Description	Image
<ul style="list-style-type: none"> Used with the torque wrench for adjustment of the final implant placement Yellow grooves aligns with abutment hex direction Match the groove of OneGuide template with the groove of driver *C = Connection 	
*C	Mini (Ø3.4)
F3.0	HOGFDM35

Adapter	
Description/Item code	Image
<ul style="list-style-type: none"> Use as a torque driver to connecting to the engine 	
TEADT	

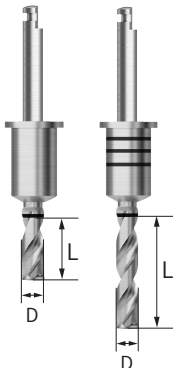
OneMS Path Drill			
Description		Image	
<ul style="list-style-type: none"> Used for correcting path deviation Can establish implant placement path during surgery For inclined bone cutting with a flat blade design For the 13mm specification, depth adjustment follows marking lines: upper line (11.5mm), middle line (10mm), lower line (8.5mm) Recommended speed: 1,200~1,500 rpm 			
L	D/Ø	Ø1.5	Ø2.0
7.0		HOMSD1507	HOMSD2007
13.0		HOMSD1513	HOMSD2013

Drilling Sequence OneMS Drill


EKIII | ETIII | EM(MS)

(Length: 8.5mm)


MS Ø2.0/Ø2.5

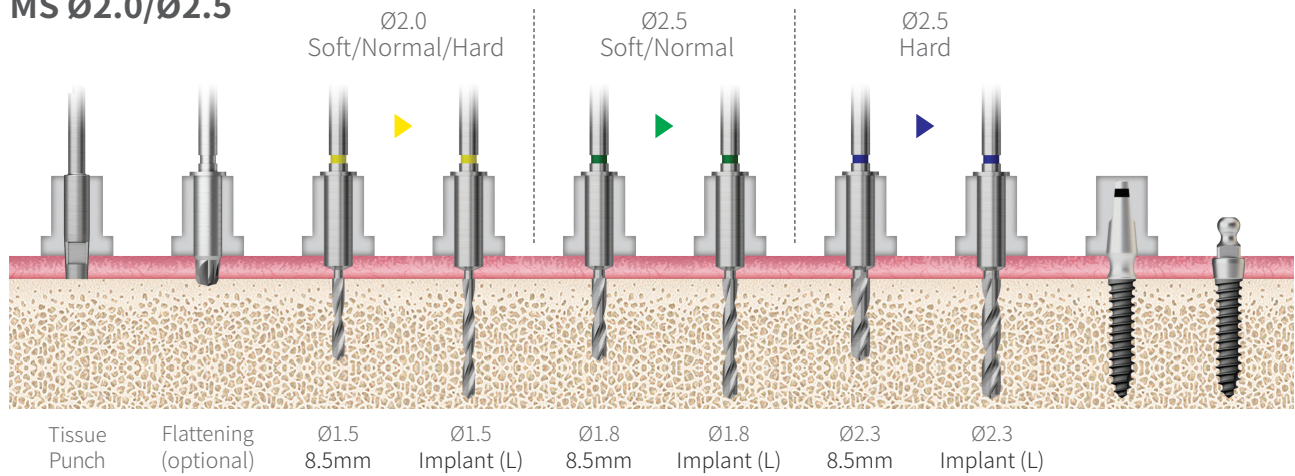

MS Ø3.0

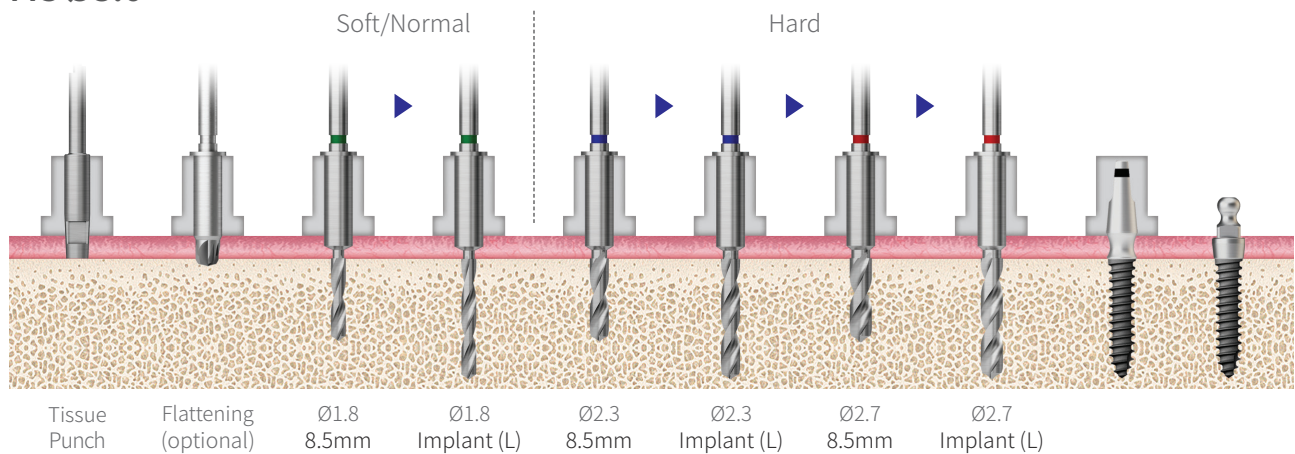

ETIII Ø3.2

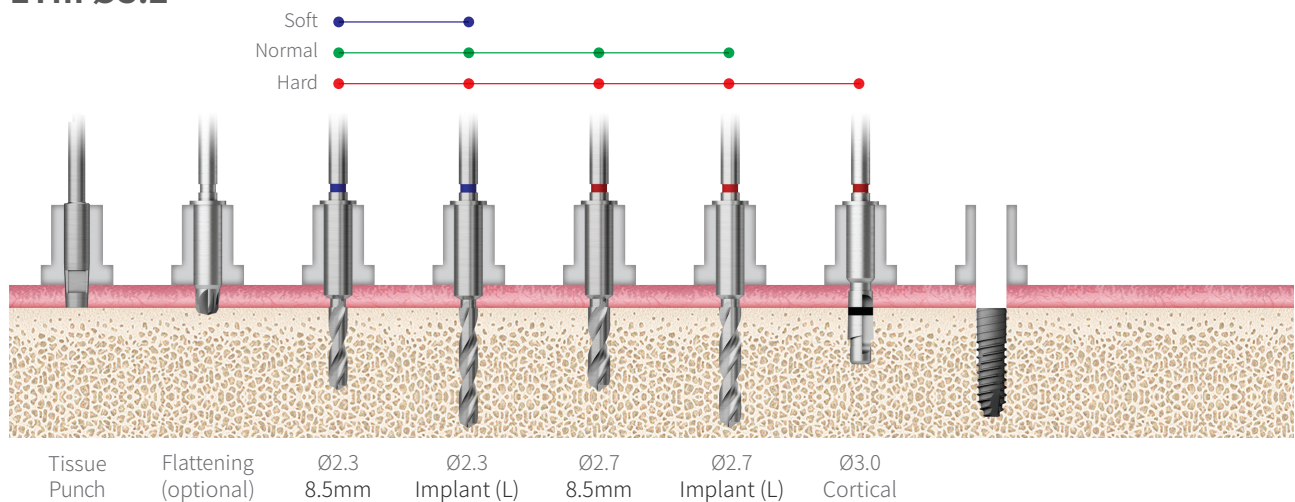

122 Taper Kit (H122TPK)

※ 122 Taper (EK) Kit: HK122TPK

For

EKIII

ETIII/IV


SSIII

Top panel components


Torque Wrench
TQWCB






Depth Gauge
ODG

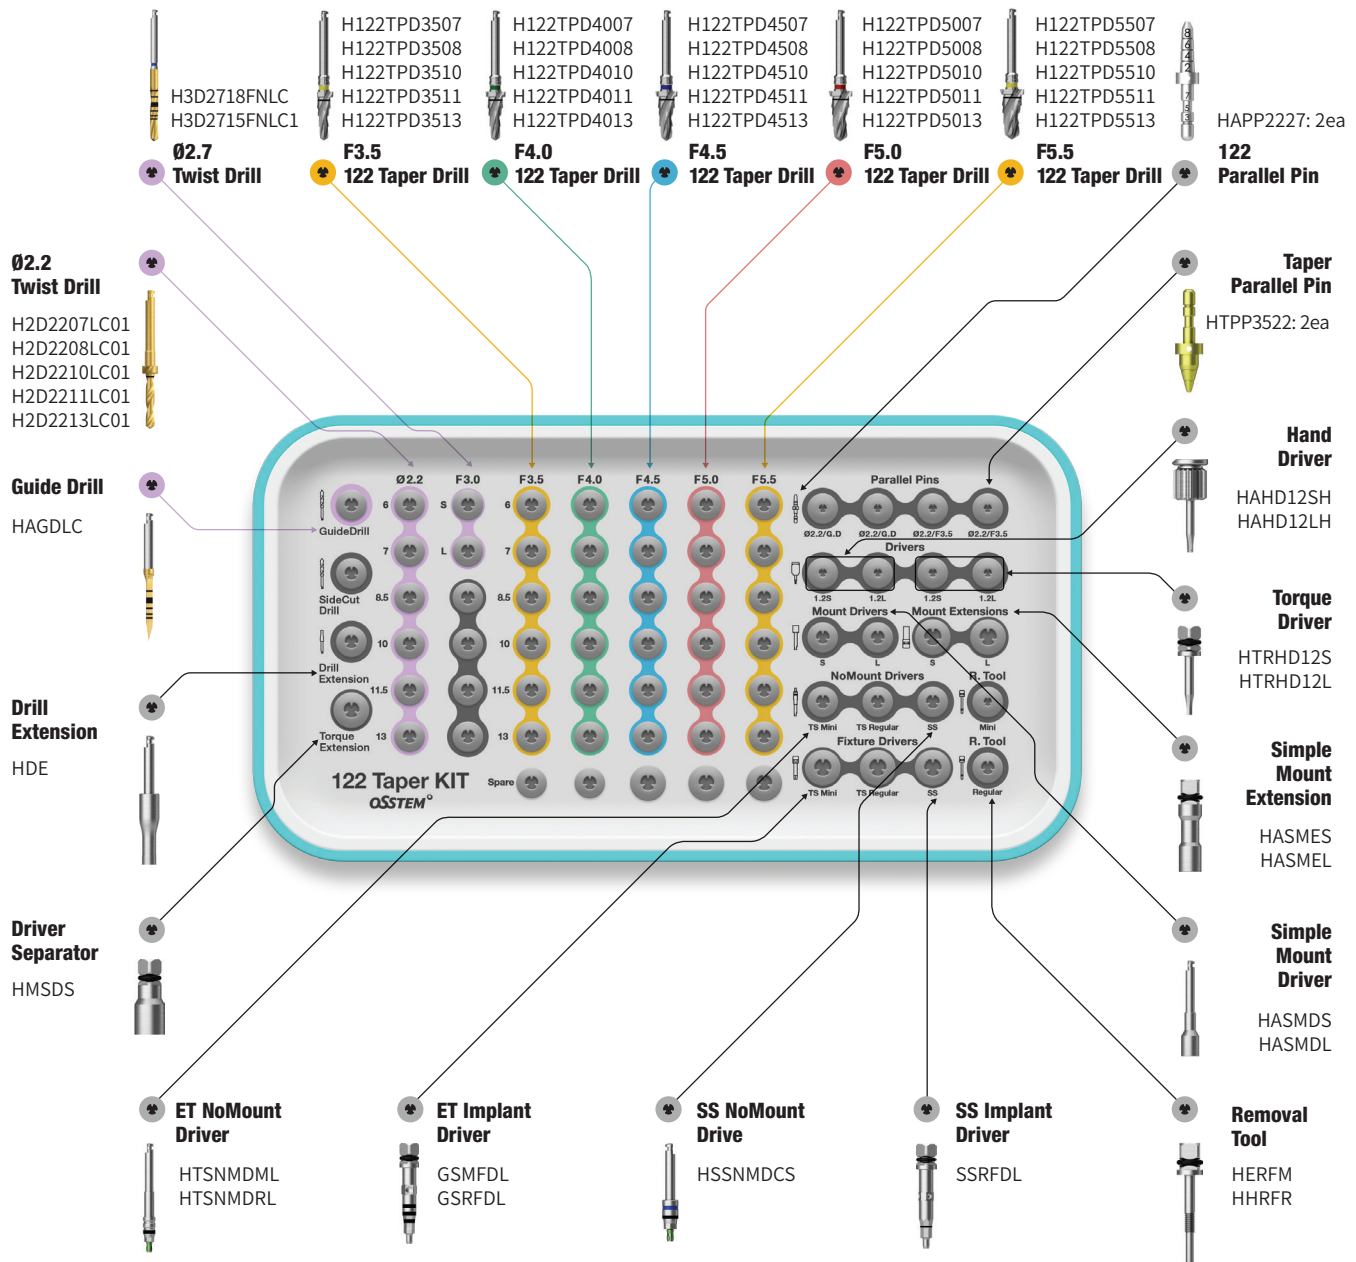

122 Taper Kit Surgical Kit Instruments

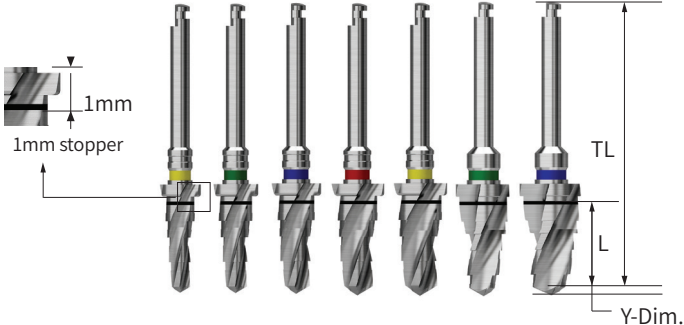122 Taper Drill									
Description				Image/Guide					
<ul style="list-style-type: none"> Taper drill for Type III implants Specification by diameter and length Color coding displays implant diameter One step large-diameter drill is used to remove cortical bone from the hard bone 122 Taper Kit single item (excluded from Taper Kit) 									
L	TL	D/Ø Y-Dim.	F3.5 0.7	F4.0 0.9	F4.5 1.0	F5.0 1.0	F5.5 1.0	F6.0 1.0	F7.0 1.0
4.0	29.5		H122TPD3504	H122TPD4004	H122TPD4504	H122TPD5004	H122TPD5504	-	-
5.0	29.5		H122TPD3505	H122TPD4005	H122TPD4505	H122TPD5005	H122TPD5505	-	-
6.0	30.5		H122TPD3506	H122TPD4006	H122TPD4506	H122TPD5006	H122TPD5506	H122TPD6006	H122TPD7006
7.0	31.5		H122TPD3507	H122TPD4007	H122TPD4507	H122TPD5007	H122TPD5507	H122TPD6007	H122TPD7007
8.5	33		H122TPD3508	H122TPD4008	H122TPD4508	H122TPD5008	H122TPD5508	H122TPD6008	H122TPD7008
10	34.5		H122TPD3510	H122TPD4010	H122TPD4510	H122TPD5010	H122TPD5510	H122TPD6010	H122TPD7010
11.5	34.5		H122TPD3511	H122TPD4011	H122TPD4511	H122TPD5011	H122TPD5511	H122TPD6011	H122TPD7011
13	36		H122TPD3513	H122TPD4013	H122TPD4513	H122TPD5013	H122TPD5513	H122TPD6013	H122TPD7013
15	38		H122TPD3515	H122TPD4015	H122TPD4515	H122TPD5015	H122TPD5515	-	-
Color			Yellow	Green	Blue	Red	Yellow	Green	Blue

Cortical Drill for Ultra-Wide			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Drill is used to remove cortical bone from hard bone (for ultra-wide) Dedicated drill by implant diameter It is recommended to drill to the bottom line of the marking line 	F6.0	HCD4C60	
	F7.0	HCD4C70	


Parallel Pin for 122 Taper Drill		
Description	Item Code	Image
<ul style="list-style-type: none"> Parallel pin for 122 Taper Drill Used for checking position and direction of bone preparation Lower part for 2.2 drill, upper part for guide drill 122 Taper Kit single item (excluded from Taper Kit) Other components same as Taper Kit 	HAPP2227	

Drilling Sequence **122 Taper Drill**


EKIII | ETIII | SSIII

(Length: 10mm)


Ø3.0mm

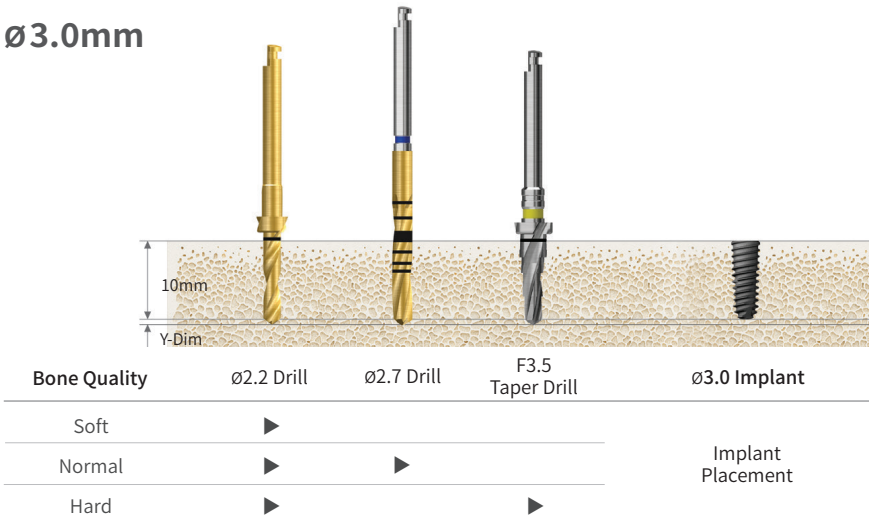


Ø3.5mm

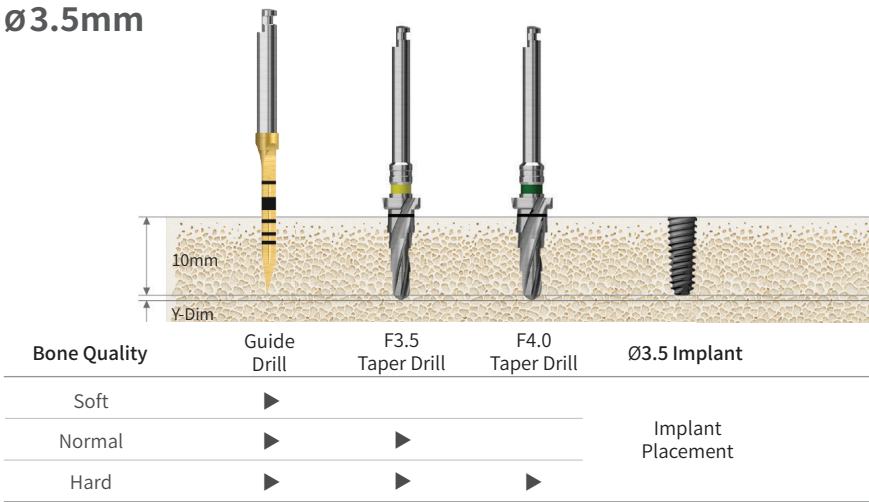

Ø4.0mm

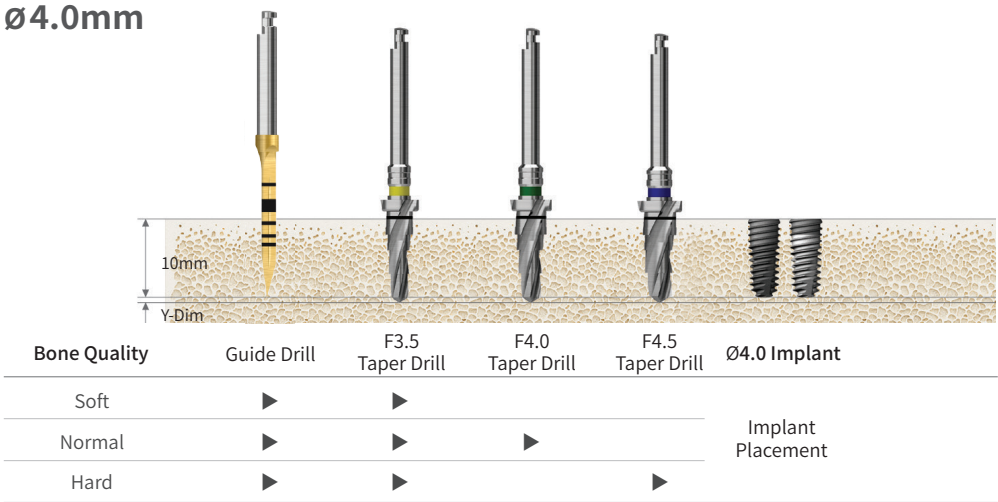


Ø4.5mm

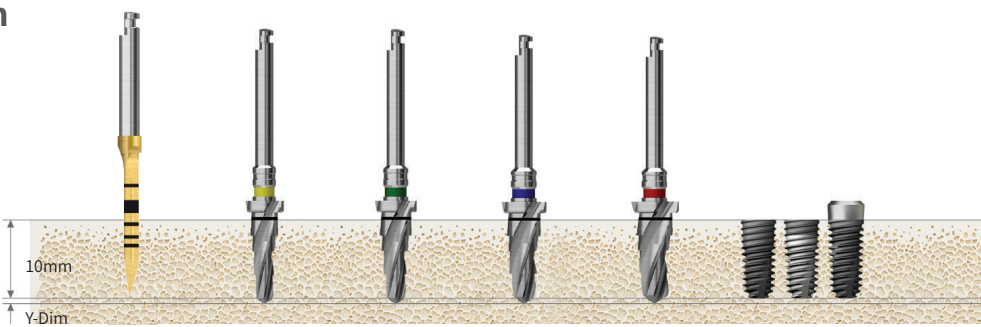


Bone Quality	Guide Drill	F3.5 Taper Drill	F4.0 Taper Drill	F4.5 Taper Drill	F5.0 Taper Drill	Ø4.5 Implant
Soft	▶		▶			Implant Placement
Normal	▶	▶		▶		
Hard	▶	▶			▶	

Ø5.0mm

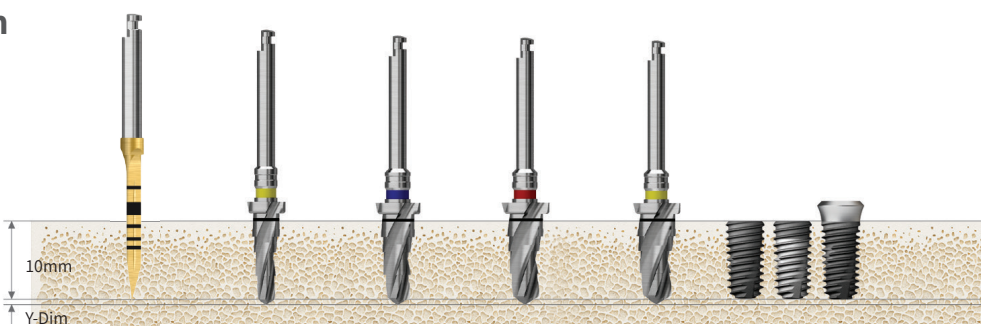

Bone Quality	Guide Drill	F3.5 Taper Drill	F4.5 Taper Drill	F5.0 Taper Drill	F5.5 Taper Drill	Ø5.0 Implant
Soft	▶		▶			Implant Placement
Normal	▶	▶		▶		
Hard	▶	▶			▶	

Ø5.5mm

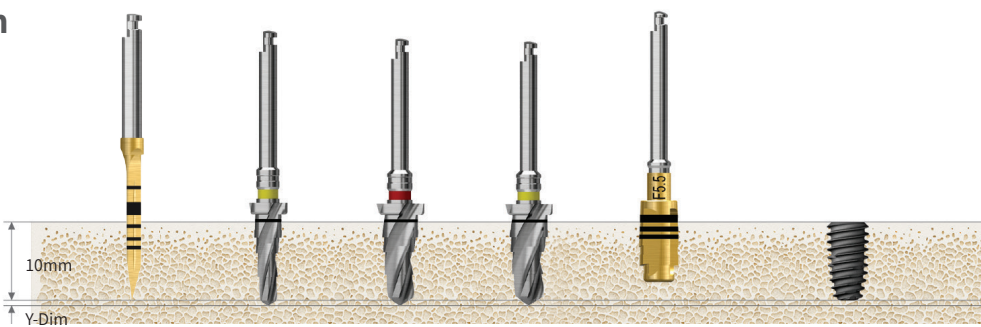

Bone Quality	Guide Drill	F3.5 Taper Drill	F5.0 Taper Drill	F5.5 Taper Drill	F5.5 Taper Cortical Drill	Ø5.5 Implant
Soft	▶		▶			Implant Placement
Normal	▶	▶		▶		
Hard	▶	▶		▶	▶	

F5.5 taper cortical drill marking line: bottom line 6mm or less, middle line 7mm, top line 8.5mm or more

Recommended insertion torque $\leq 40\text{Ncm}$. ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.

(Length: 10mm)

Ø7.0mm

10mm

Y-Dim

Bone Quality	Guide Drill	F3.5 Taper Drill	F5.0 Taper Drill	F6.0 Taper Drill	F7.0 Taper Drill	F7.0 Cortical Drill	Ø7.0 Implant
Soft	▶		▶	▶			Implant Placement
Normal	▶	▶	▶		▶		
Hard	▶	▶	▶		▶	▶	


Recommended insertion torque $\leq 40\text{Ncm}$. ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.

Drilling Sequence **122 Taper Drill**

ETIV


(Length: 10mm)

Ø4.0mm

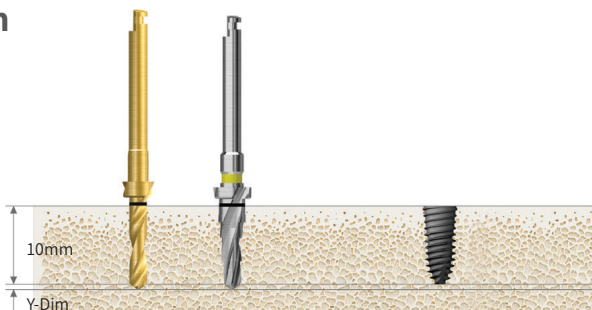


Bone Quality	Ø2.2 Drill	F3.5 Taper Drill	Ø4.0 Implant
D4	▶		Implant Placement
Soft	▶	▶	

Ø4.5mm

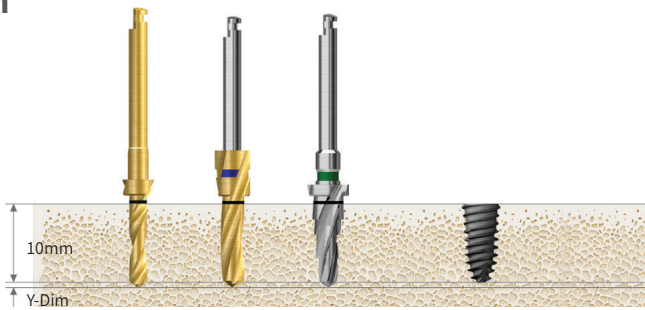

Bone Quality	Ø2.2 Drill	Ø3.0 Drill	F4.0 Taper Drill	Ø4.5 Implant
D4		▶		Implant Placement
Soft	▶		▶	

Ø5.0mm

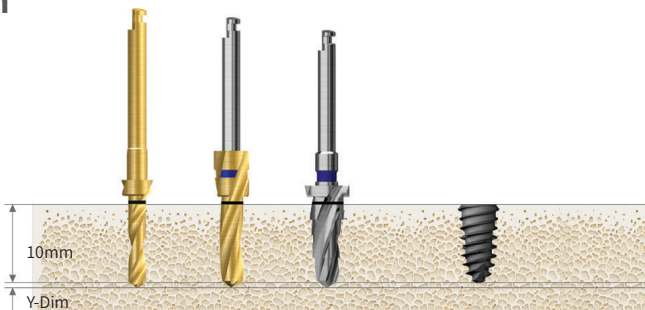

Bone Quality	Ø2.2 Drill	Ø3.0 Drill	F4.5 Taper Drill	Ø5.0 Implant
D4		▶		Implant Placement
Soft	▶		▶	


Drilling Sequence

122 Taper Drill


ETIV Ultra-wide

(Length: 10mm)

Ø6.0mm

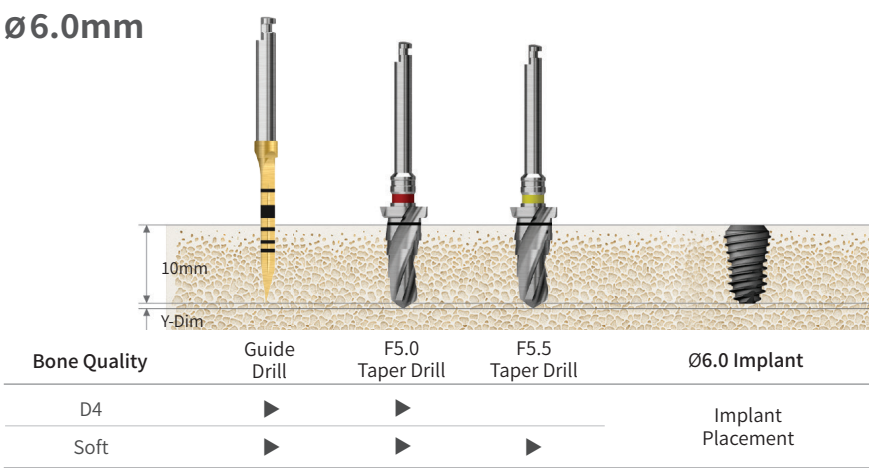

Ø7.0mm

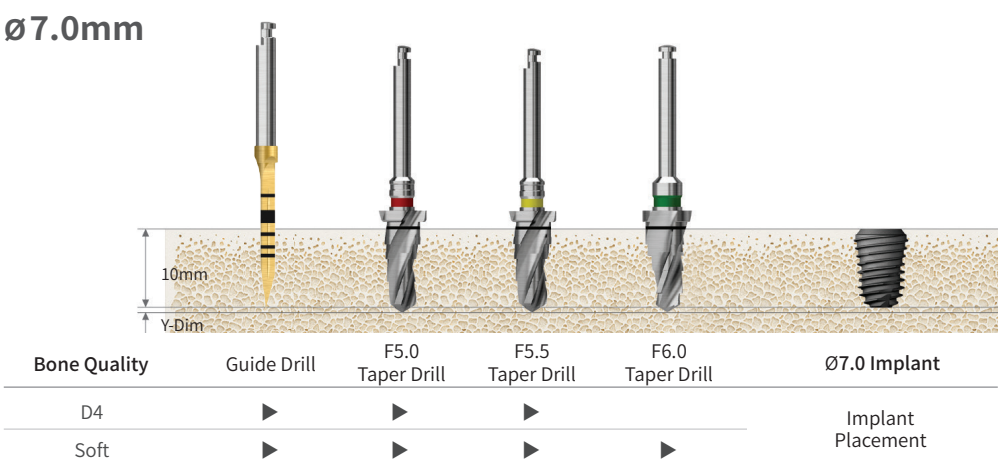

F5.5 taper cortical drill marking line: bottom line 6mm or less, middle line 7mm, top line 8.5mm or more
 Recommended insertion torque ≤40Ncm. ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.



Taper Kit (HTAPEK)

※ Taper (EK) Kit: **HKTAPEK**

For

EKIII

ETIII/IV


SSIII

Top panel components

Torque Wrench
TQWCB



Depth Gauge
ODG

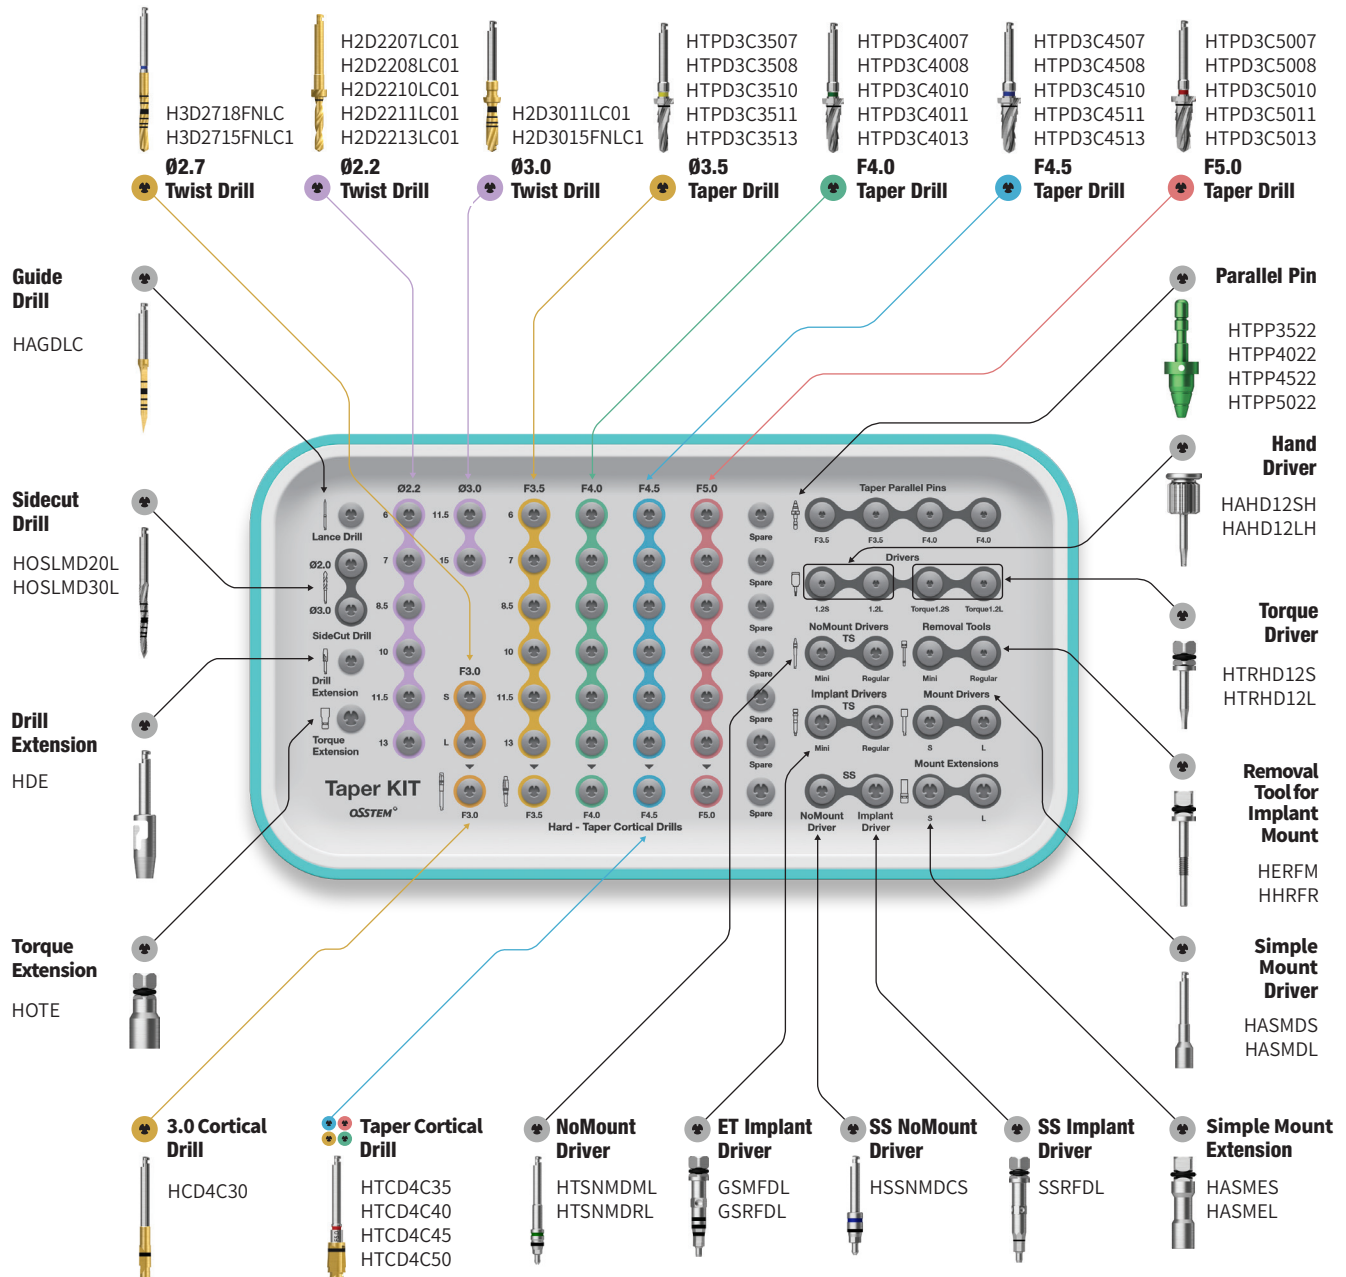

Taper Ultra Kit (HULTPK)


For **Ultra-wide**

Top panel components

Open Wrench
SPOW



Ratchet Wrench
RCWC

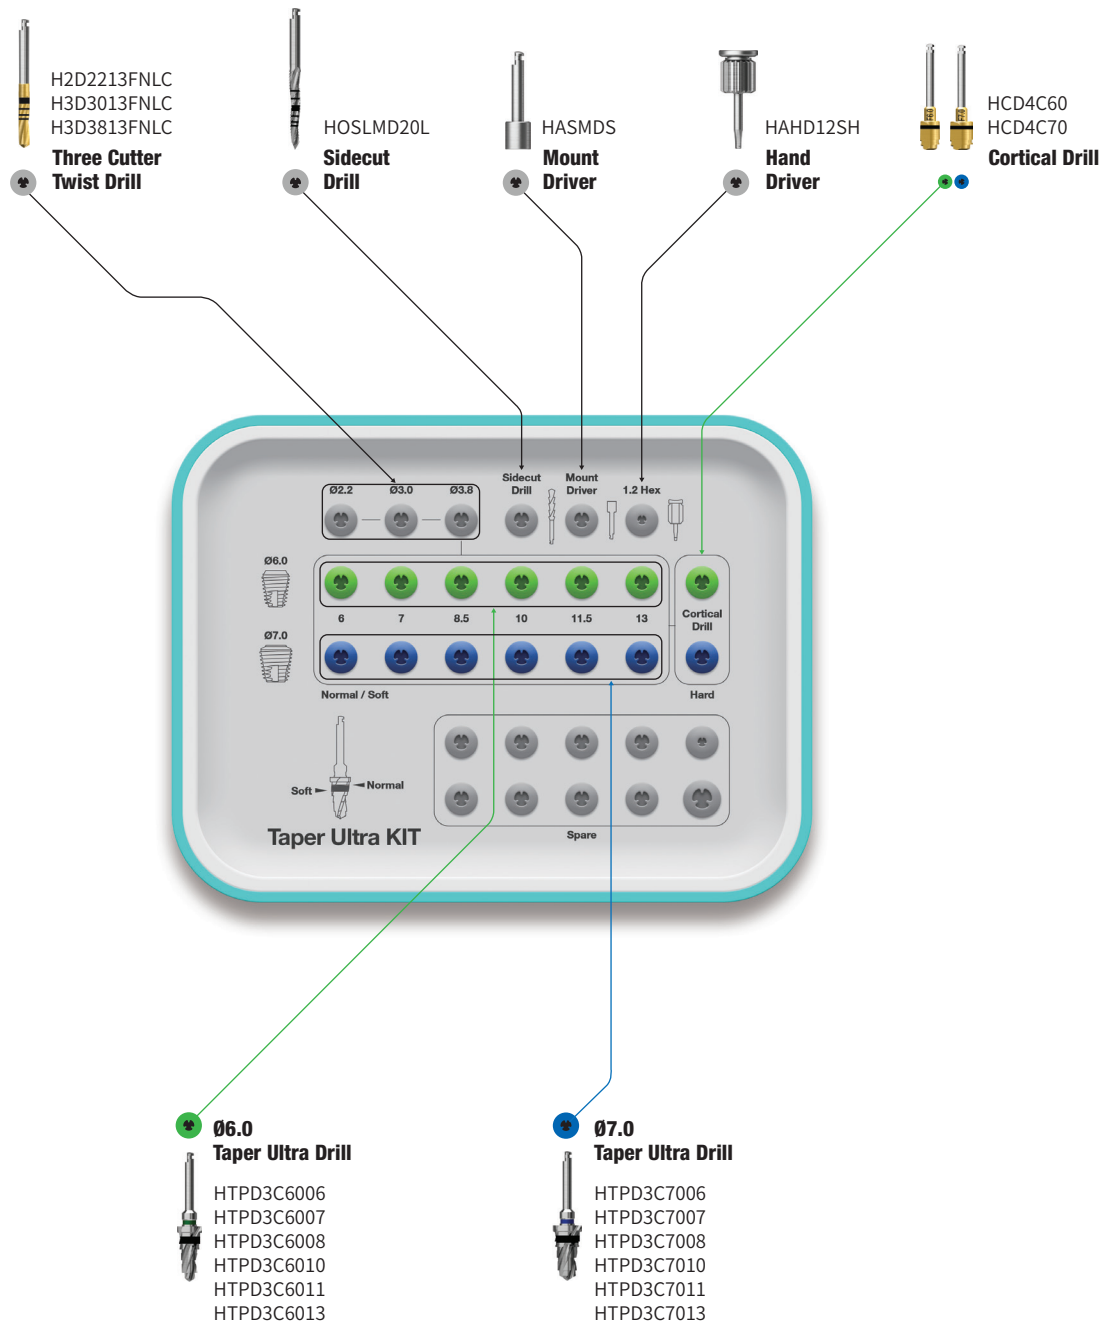

Taper Kit Surgical Kit Instruments

Taper Drill							
Description			Image/Guide				
<ul style="list-style-type: none"> Taper drill for taper(III type) implant by diameter and length Stopper drill with 1mm space Color coding displays implant diameter F3.5: yellow, F4.0: green, F4.5: blue, F5.0: red, F5.5: yellow Taper Kit single item (*excluded from 122 Taper Kit) 							
L	TL	D/Ø Y-Dim.	F3.5	F4.0	F4.5	F5.0	F5.5
5.0	29.5		HTPD3C3505	HTPD3C4005	HTPD3C4505	HTPD3C5005	-
6.0	30.5		HTPD3C3506	HTPD3C4006	HTPD3C4506	HTPD3C5006	HTPD3C5506
7.0	31.5		HTPD3C3507	HTPD3C4007	HTPD3C4507	HTPD3C5007	HTPD3C5507
8.5	33		HTPD3C3508	HTPD3C4008	HTPD3C4508	HTPD3C5008	HTPD3C5508
10	34.5		HTPD3C3510	HTPD3C4010	HTPD3C4510	HTPD3C5010	HTPD3C5510
11.5	34.5		HTPD3C3511	HTPD3C4011	HTPD3C4511	HTPD3C5011	HTPD3C5511
13	36		HTPD3C3513	HTPD3C4013	HTPD3C4513	HTPD3C5013	HTPD3C5513
15	38		HTPD3C3515	HTPD3C4015	HTPD3C4515	HTPD3C5015	HTPD3C5515
Color			Yellow	Green	Blue	Red	Yellow

Taper Cortical Drill for Taper Implant (ETIII, SSIII, USIII)			
Description	D/Ø	Item code	Image
<ul style="list-style-type: none"> The drill is used to remove cortical bone of the hard bone (used right after the use of Taper Drill) Dedicated drill for each implant diameter F3.5~5.0 drill marking line: bottom line 8.5mm or less, top line 10mm or more implant placement standard F5.5 drill marking line: bottom line 6mm or less, middle line 7mm, top line 8.5mm or more implant placement standard It is recommended to drill to the bottom of the marking line Taper Kit single item (excluded from 122 Taper Kit) 	F3.5	HTCD4C35	
	F4.0	HTCD4C40	
	F4.5	HTCD4C45	
	F5.0	HTCD4C50	
	F5.5	HTCD4C55	

Taper Ultra Drill				
Description	L	F6.0	F7.0	Image
<ul style="list-style-type: none"> Taper drill for taper ultra-wide implant by diameter and length Stopper drill with 1mm space Color coding displays implant diameter 	6.0	HTPD3C6006	HTPD3C7006	
	7.0	HTPD3C6007	HTPD3C7007	
	8.5	HTPD3C6008	HTPD3C7008	
	10	HTPD3C6010	HTPD3C7010	
	11.5	HTPD3C6011	HTPD3C7011	
	13	HTPD3C6013	HTPD3C7013	
	Color	Green	Blue	

Parallel Pin for Taper Drill			
Description	D/Ø	Item code	Image
<ul style="list-style-type: none"> Parallel pin for taper drill Used for checking position and direction of bone preparation The lower part is for implant diameter drill and the upper part is for initial drill Color coding by implant diameter (F3.5: yellow, F4.0: green, F4.5: blue, F5.0: silver) 122 Taper & Taper Kit common components 	F3.5	HTPP3522	
	F4.0	HTPP4022	
	F4.5	HTPP4522	
	F5.0	HTPP5022	

Cortical Drill for Ultra-Wide			
Description	D/Ø	Item code	Image
<ul style="list-style-type: none"> The drill is used to removing cortical bone at the hard bone (for ultra-wide) Dedicated drill for each implant diameter It is recommended to drill to the bottom of the marking line 	F6.0	HCD4C60	
	F7.0	HCD4C70	


Tapered Implant Tap for ETIII, USIII, SSIII			
Description	D/Ø	Item code	Image
<ul style="list-style-type: none"> Tap for tapered implant (III type) Used in hard bone and forming implant screw thread Engine (25rpm recommended) or torque wrench after mount extension fastening Tapping to the bottom of the marking line is recommended (for F5.0, the bottom line below 7.0mm implant and the upper line over 8.5mm implant placement standard) 	F3.5	HFTS35	
	F4.0	HFTS40	
	F4.5	HFTS45	
	F5.0	HFTS50	

Drilling Sequence **Taper Drill**

EKIII | ETIII | SSIII


(Length: 10mm)

Ø3.2mm

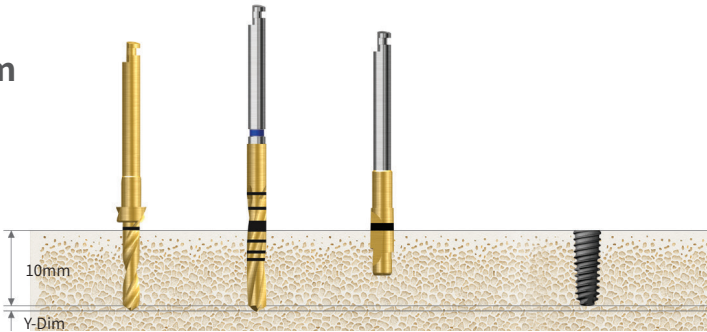


Bone Quality	Ø2.2 Drill	Ø2.7 Drill	F3.0 Cortical Drill	Ø3.0 Implant
Soft	▶			Implant Placement
Normal	▶	▶		
Hard	▶	▶	▶	

Ø3.5mm

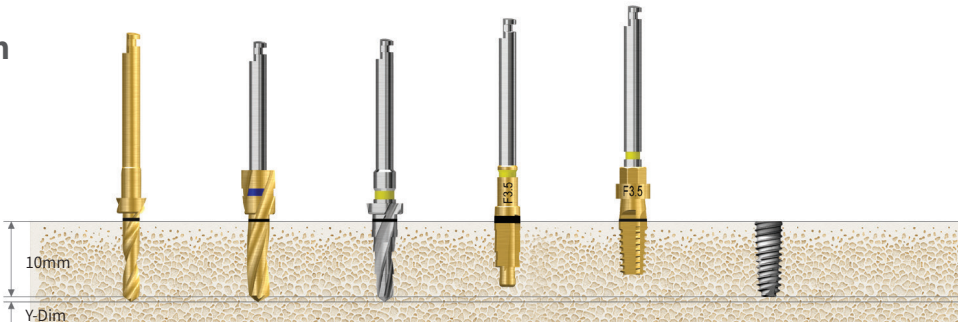


Bone Quality	Ø2.2 Drill	Ø3.0 Drill	F3.5 Taper Drill	F3.5 Taper Cortical Drill	F3.5 Taper Implant Tap	Ø3.5 Implant
Soft	▶	▶				Implant Placement
Normal	▶		▶			
Hard	▶		▶	▶		
Hard (Option)	▶		▶		▶	

Ø4.0mm

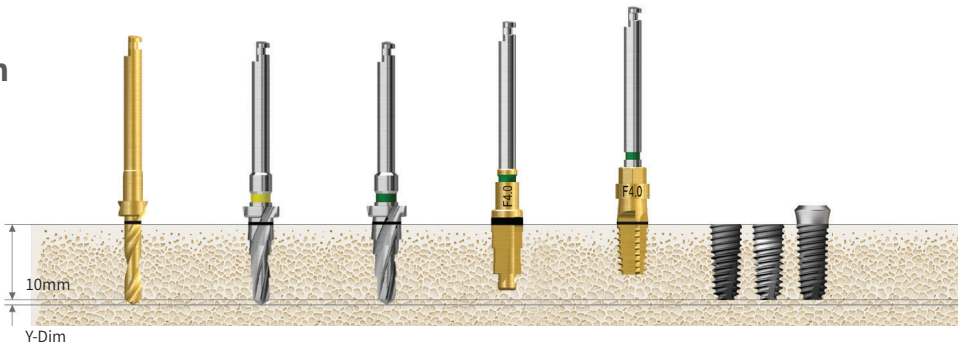

Bone Quality	Ø2.2 Drill	F3.5 Taper Drill	F4.0 Taper Drill	F4.0 Taper Cortical Drill	F4.0 Taper Implant Tap	Ø4.0 Implant
Soft	▶	▶				Implant Placement
Normal	▶	▶	▶			
Hard	▶	▶	▶	▶		
Hard (Option)	▶	▶	▶		▶	


Ø4.5mm

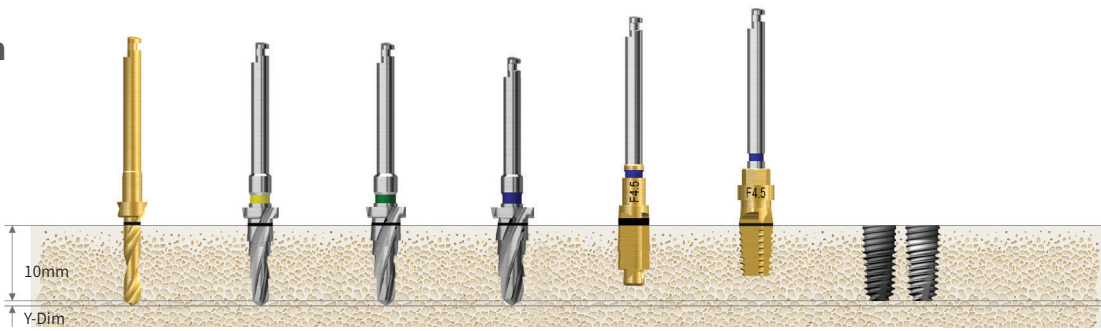

Bone Quality	Ø2.2 Drill	F3.5 Taper Drill	F4.0 Taper Drill	F4.5 Taper Drill	F4.5 Taper Cortical Drill	F4.5 Taper Implant Tap	Ø4.5 Implant
Soft	▶	▶	▶				
Normal	▶	▶		▶			
Hard	▶	▶		▶	▶		
Hard (Option)	▶	▶		▶		▶	

Implant Placement


Ø5.0mm

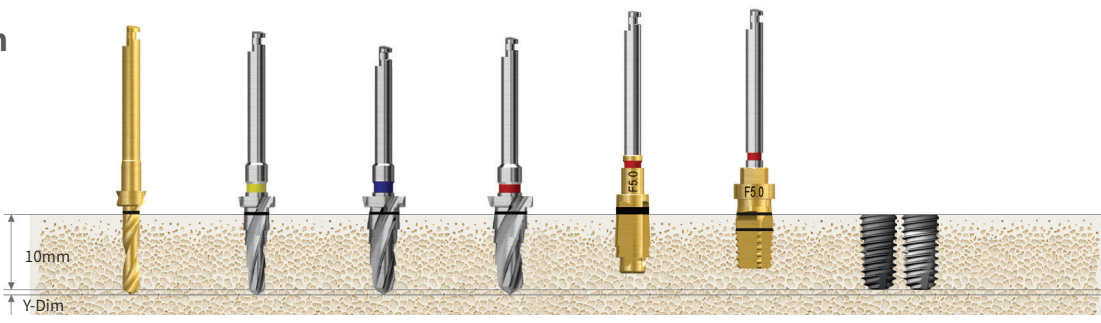

Bone Quality	Ø2.2 Drill	F3.5 Taper Drill	F4.5 Taper Drill	F5.0 Taper Drill	F5.0 Taper Cortical Drill	F5.0 Taper Implant Tap	Ø5.0 Implant
Soft	▶	▶	▶				
Normal	▶	▶	▶	▶			
Hard	▶	▶	▶	▶	▶		
Hard (Option)	▶	▶	▶	▶		▶	

Implant Placement

Ø5.5mm

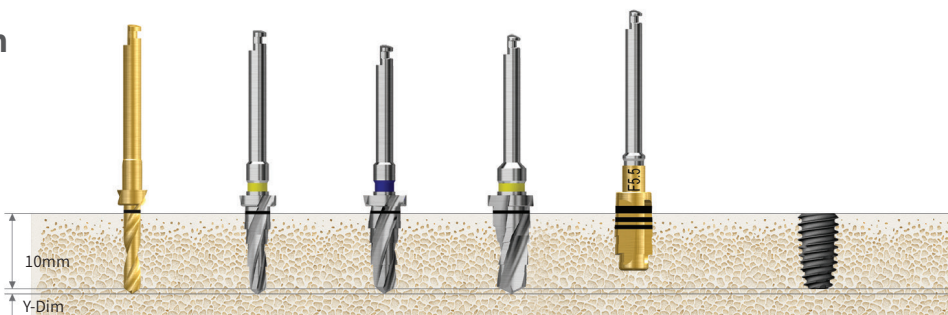

Bone Quality	Ø2.2 Drill	F3.5 Taper Drill	F4.5 Taper Drill	F5.5 Taper Drill	F5.5 Taper Implant Tap	Ø5.5 Implant
Soft	▶	▶	▶			
Normal	▶	▶	▶	▶		
Hard	▶	▶	▶	▶	▶	

Implant Placement

F5.5 taper cortical drill marking line: bottom line 6mm or less, middle line 7mm, top line 8.5mm or more

Recommended insertion torque ≤40Ncm. ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.


Implant tap used in hard bone: 25rpm recommended with engine or use with torque wrench after fastening to mount extension (F5.0 implant tap: bottom line 7mm or less, top line 8.5mm or more).

Drilling Sequence **Taper Drill**


ETIV

(Length: 10mm)


Ø4.0mm

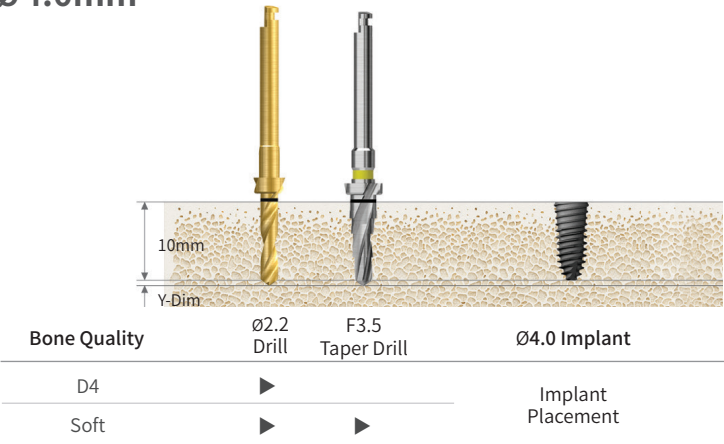

Ø4.5mm

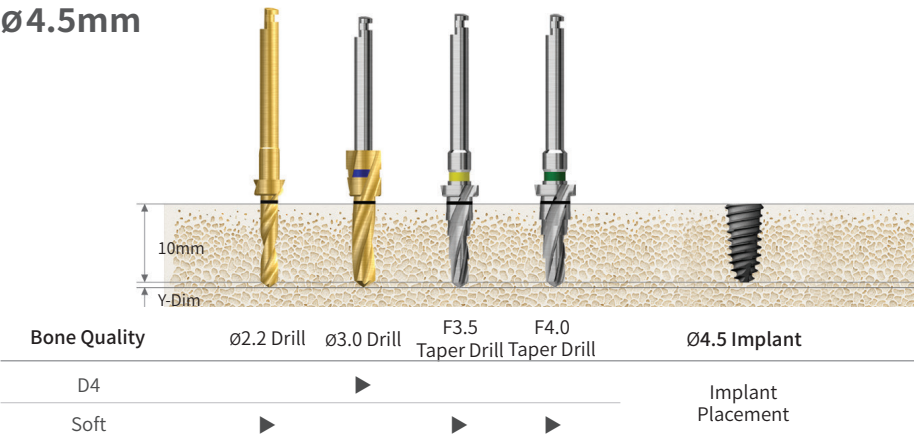

Ø5.0mm

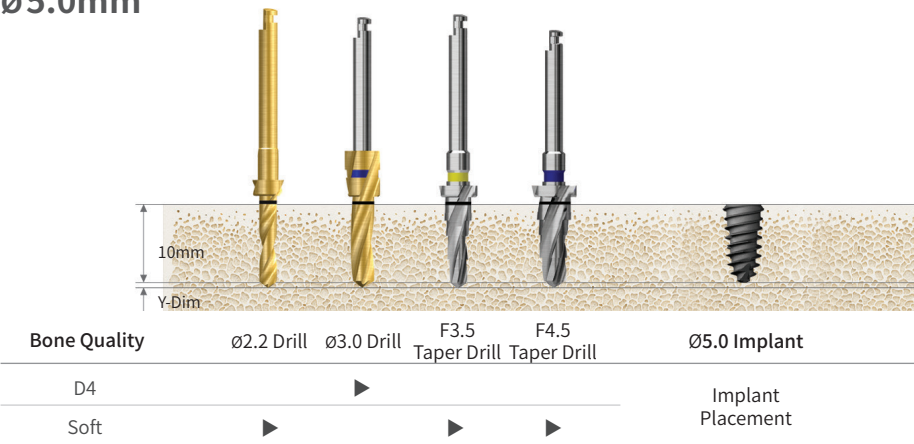


Drilling Sequence

Taper Drill


ETIII Ultra-wide

(Length: 10mm)

Ø6.0mm

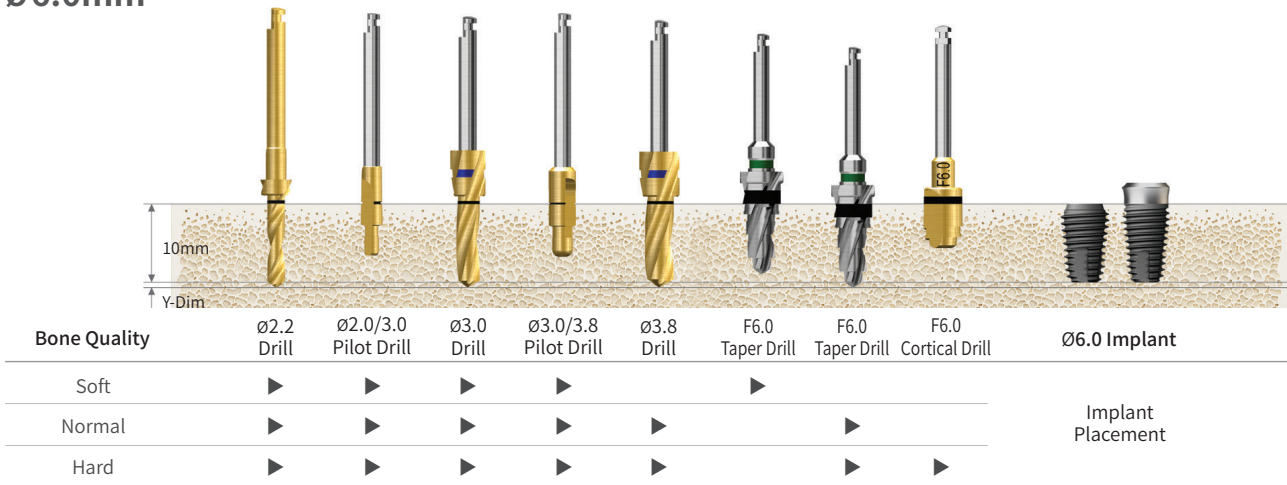

Ø7.0mm

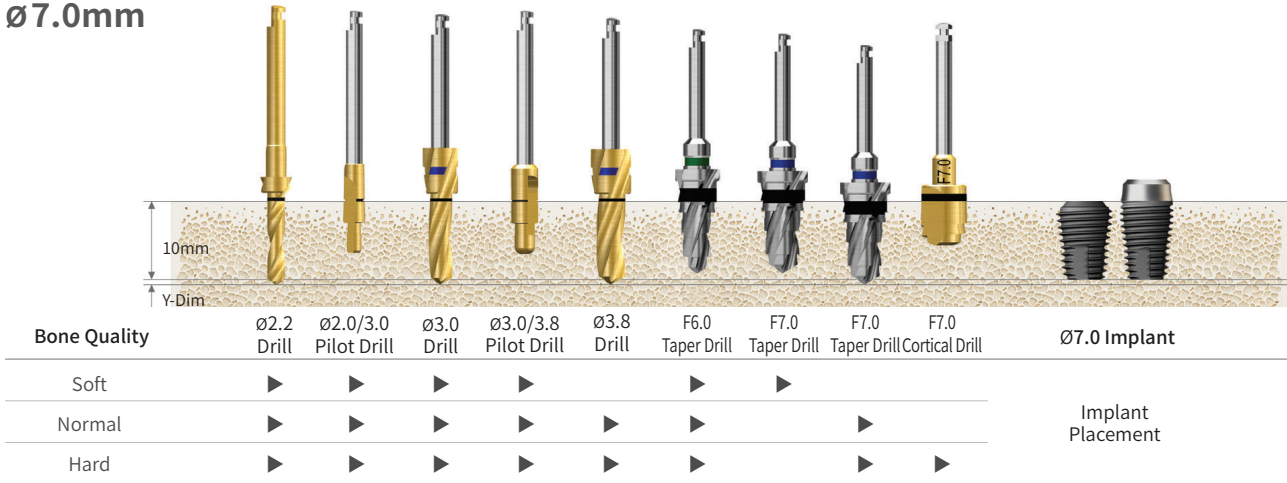

Recommended placement torque less than 40Ncm.
ET implant placement depth. The normal/hard bone is placed 1mm deeper than bone level, and the soft bone is placed at the bone level to maintain initial stability.


Drilling Sequence

Taper Drill


ETIV Ultra-wide

(Length: 10mm)

Ø6.0mm

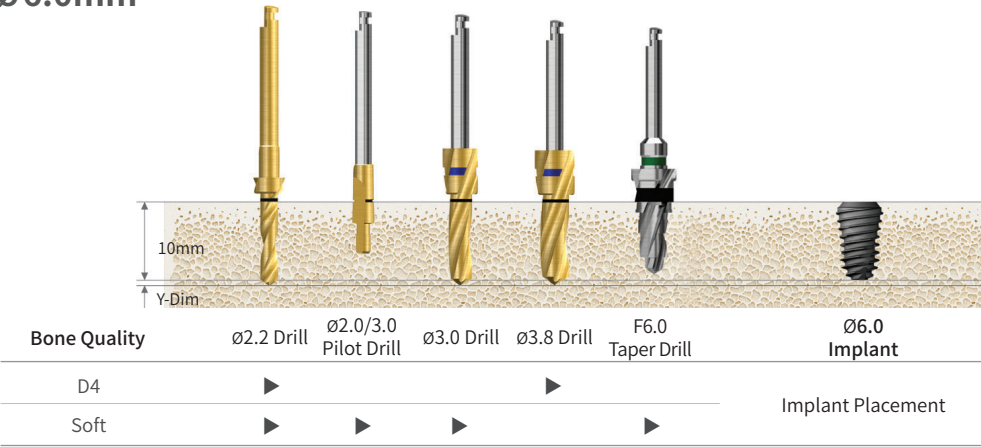

Ø7.0mm

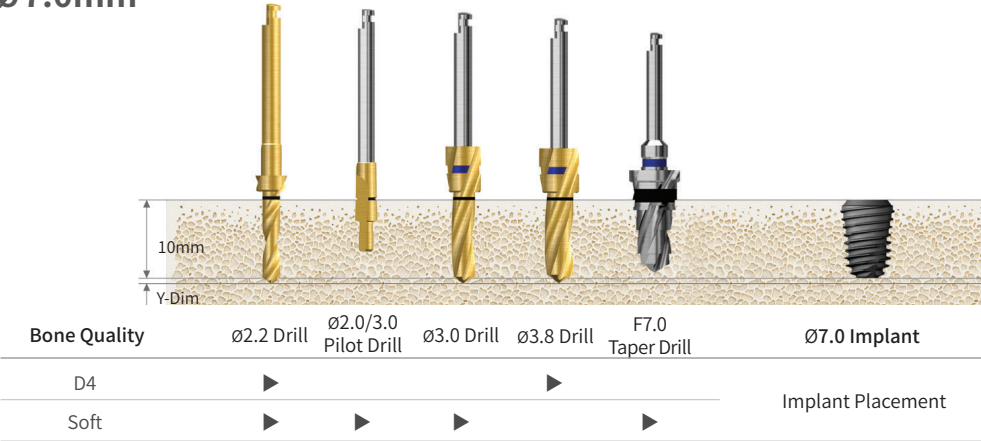

Recommended placement torque less than 40Ncm.
 ET implant placement depth. The normal/hard bone is placed 1mm deeper than bone level, and the soft bone is placed at the bone level to maintain initial stability.



485 Kit (H485K)


For EKIII ETIII/IV SSII/III Ultra-Wide

Top panel components


Torque Wrench
TQWCB




Depth Gauge
ODG

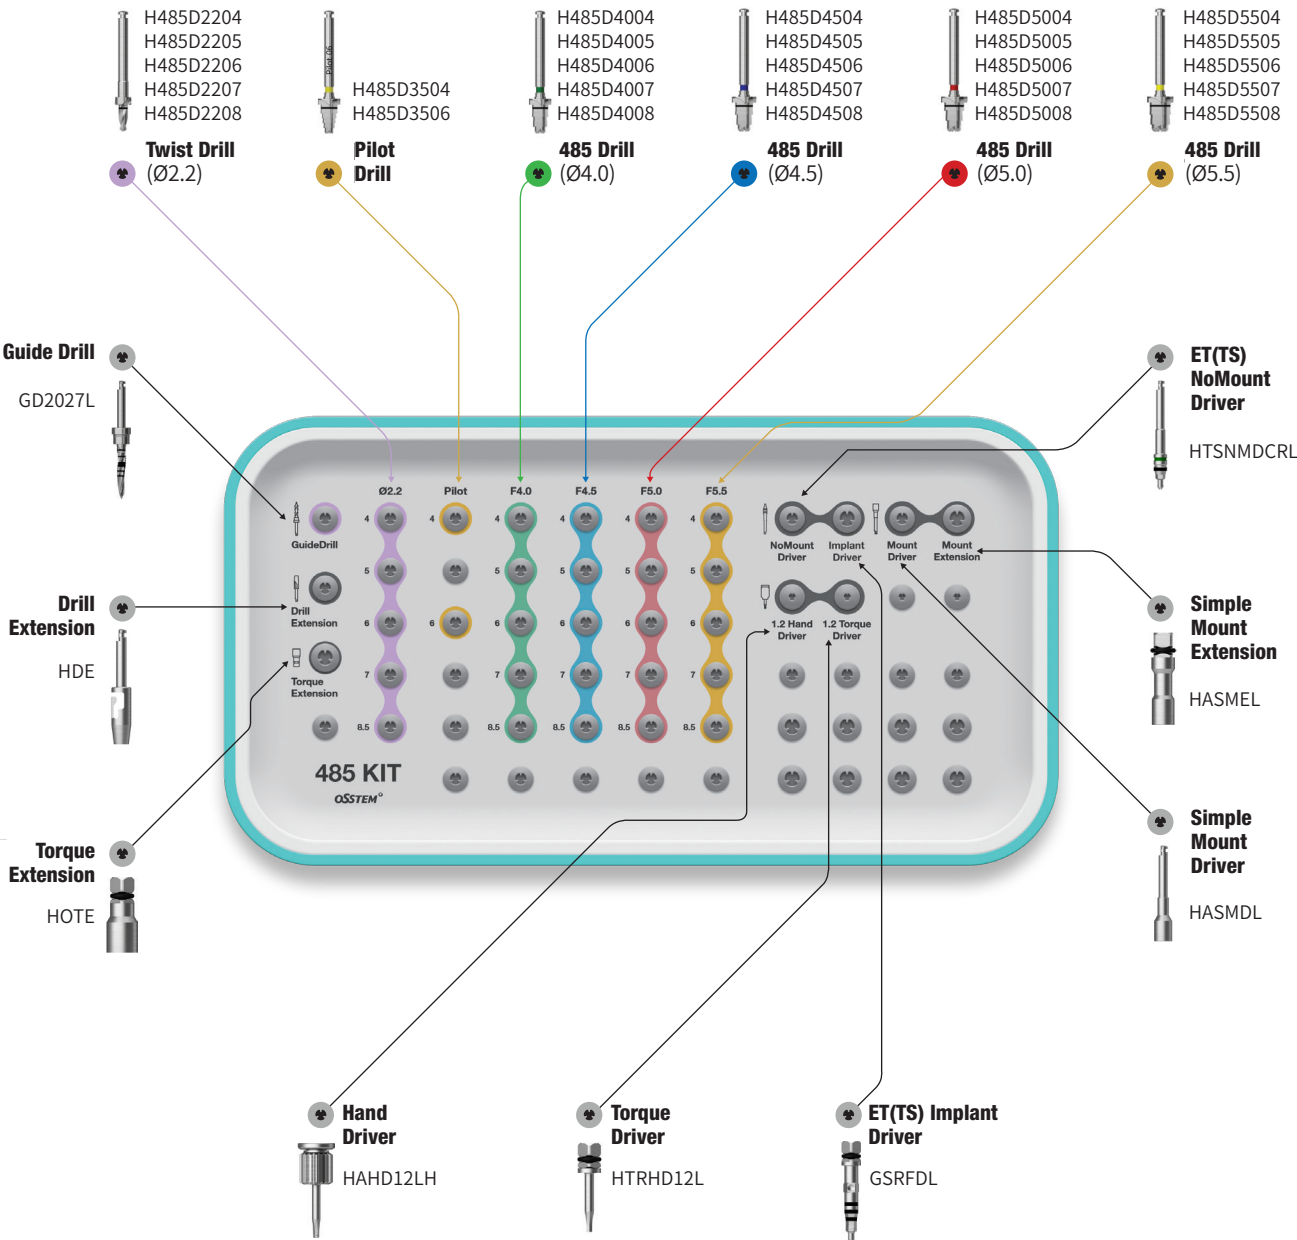

485 Kit Surgical Kit Instruments

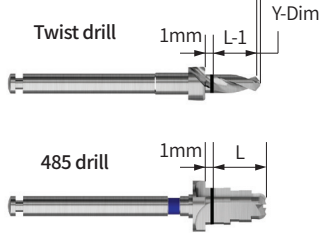485 Drill						
Description				Image/Guide		
<ul style="list-style-type: none"> Included in 485 Kit A drill for placing short implants in alveolar bone lacking in vertical dimension Ø 2.2 drill: straight drill Except for Ø 2.2 drill, the top blade of the drill is in the shape of CAS Drill, and the side blade is in the shape of taper drill A stopper drill with 1mm margin Recommended drilling speed: 800~1,200rpm 						
L	Ø2.2	Pilot	F4.0	F4.5	F5.0	F5.5
4.0	H485D2204	H485D3504	H485D4004	H485D4504	H485D5004	H485D5504
5.0	H485D2205	-	H485D4005	H485D4505	H485D5005	H485D5505
6.0	H485D2206	H485D3506	H485D4006	H485D4506	H485D5006	H485D5506
7.0	H485D2207	-	H485D4007	H485D4507	H485D5007	H485D5507
8.5	H485D2208	-	H485D4008	H485D4508	H485D5008	H485D5508

Guide Drill		
Description	Ø2.2	Image
<ul style="list-style-type: none"> Drill for marking location of osteotomy to facilitate initial drilling 	OGD2027L	

Drilling Sequence 485 Drill

EKIII

ETIII/IV

SSII/III

ULTRA-WIDE

(Length: 7mm)

Ø4.0mm

Bone Quality	Twist Drill (Ø2.2)	Pilot Drill	485 Drill (F4.0)	485 Drill (F4.5)	Ø4.0 Implant
Normal	▶	▶	▶		Implant Placement
Hard	▶	▶		▶	

Ø4.5mm

Bone Quality	Twist Drill (Ø2.2)	Pilot Drill	485 Drill (F4.5)	485 Drill (F5.0)	Ø4.5 Implant
Normal	▶	▶	▶		Implant Placement
Hard	▶	▶		▶	


Ø5.0mm

Bone Quality	Twist Drill (Ø2.2)	Pilot Drill	485 Drill (F5.0)	485 Drill (F5.5)	Ø5.0 Implant
Normal	▶	▶	▶		Implant Placement
Hard	▶	▶		▶	



Assist Kit (HOAK)

- Bone profilers are only sold in the packing unit of “Guide Screw + Bone Profiler”
- For information on the order code for ET/EK Bone Profiler, please see page 102

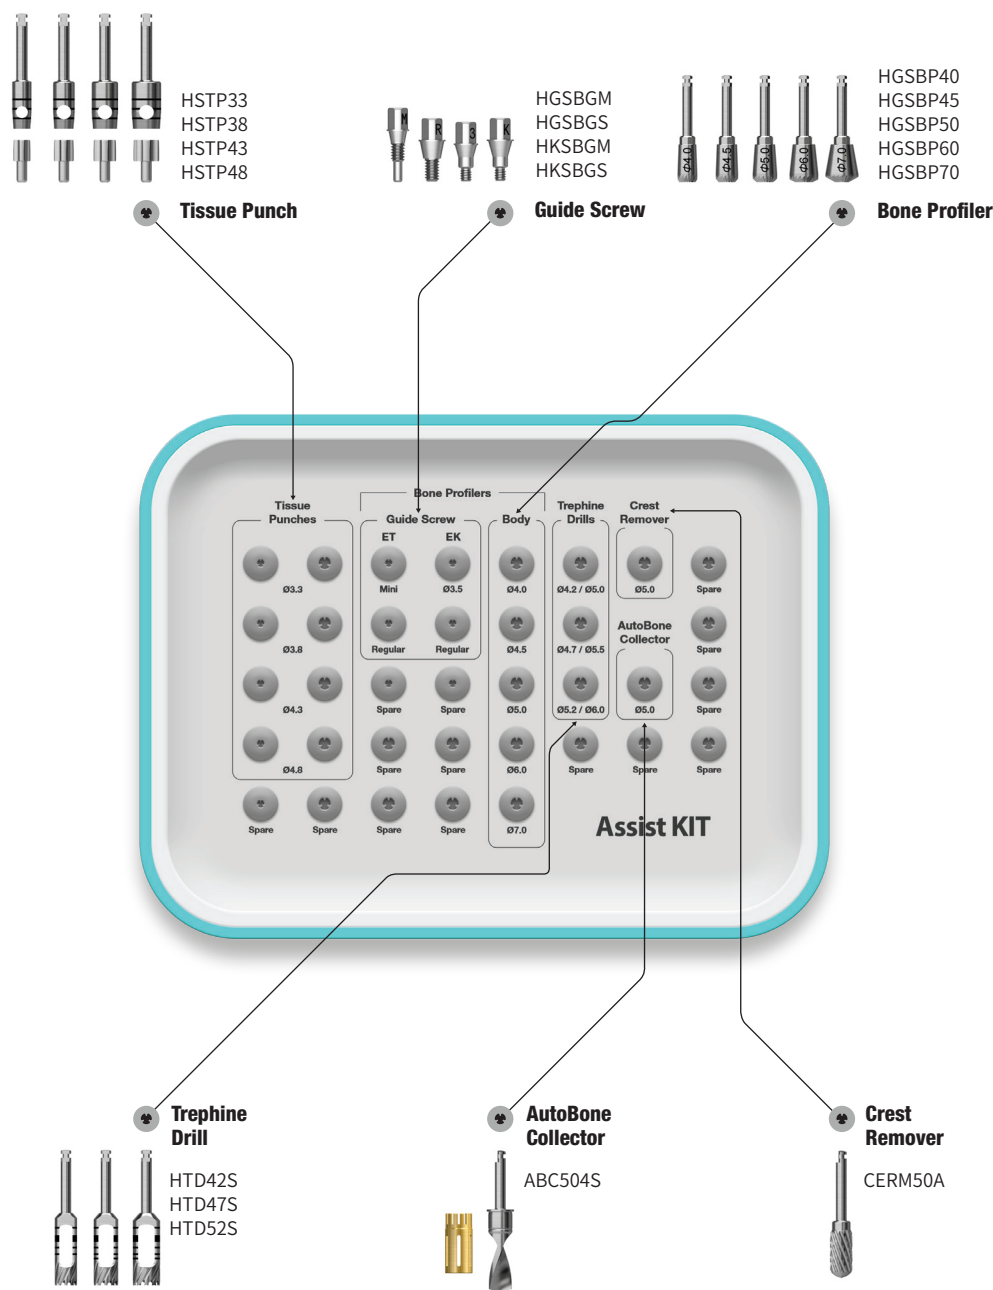



Ultra Kit (HULTRK)


For **Ultra-Wide**

Lower panel components

Open Wrench
SPOW



Ratchet Wrench
RCWC

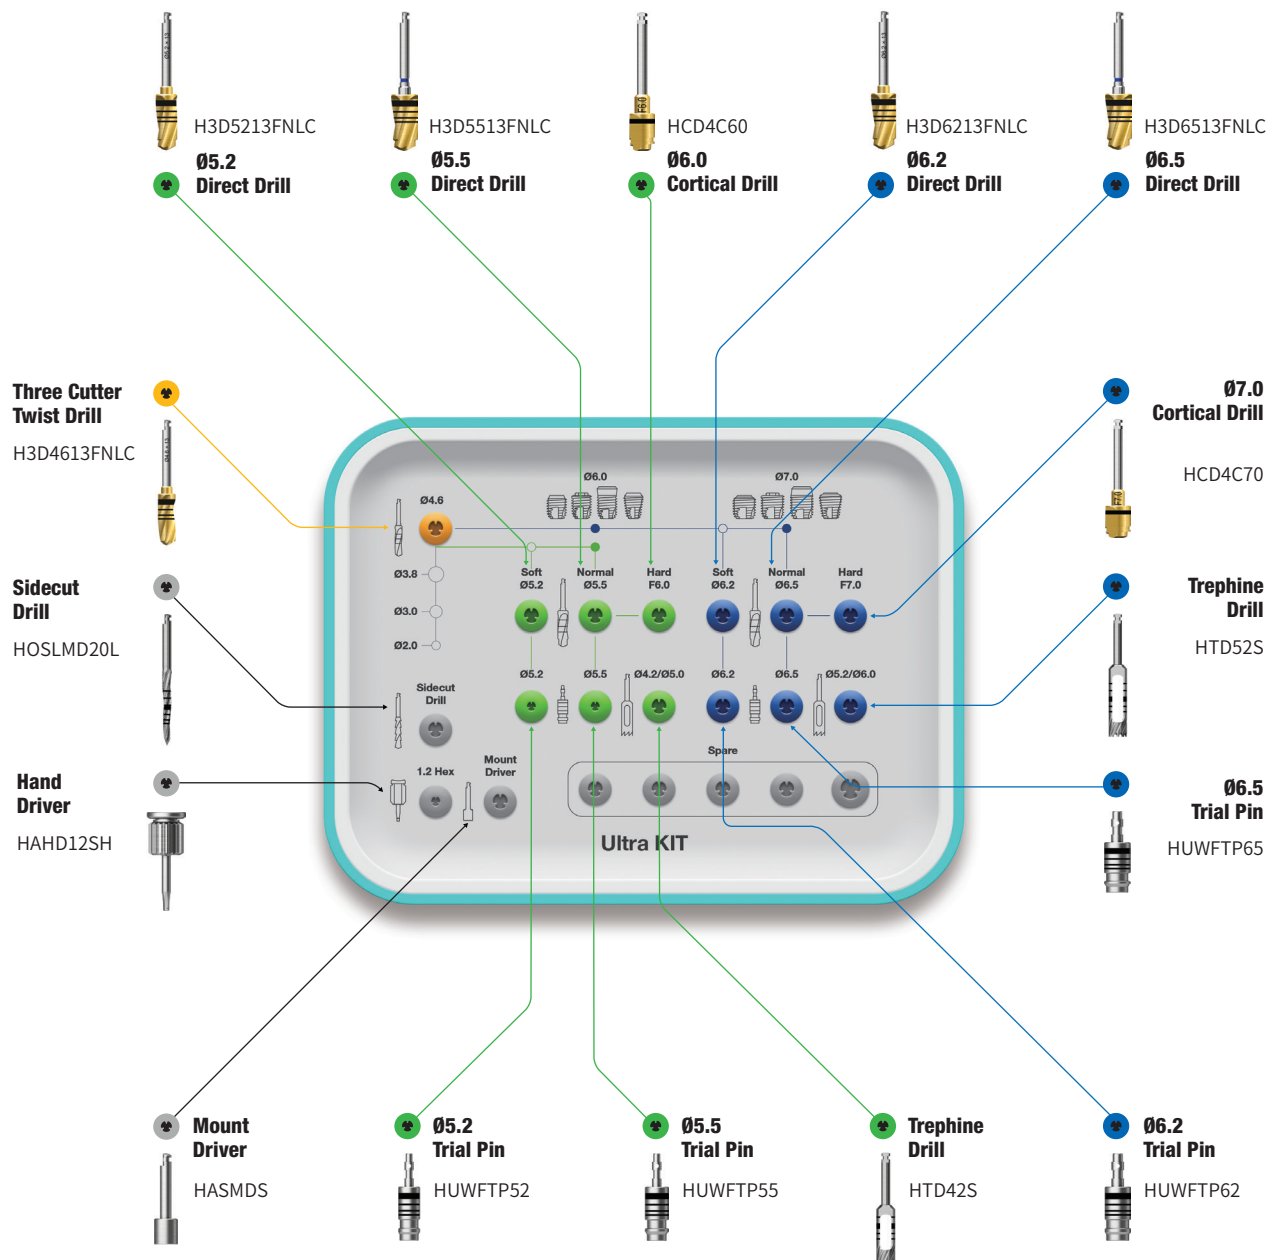

Ultra Kit Surgical Kit Instruments

Direct Drill			
Description	D1/D2	Item code	Image/Guide
<ul style="list-style-type: none"> Direct drill: two-step drill that functions like a pilot and twist drill Final drilling is possible without using pilot drill Increases initial stability in an extraction socket due to the reduced dead space at the apex 	Ø4.6/5.2	H3D5213FNLC	
	Ø4.6/5.5	H3D5513FNLC	
	Ø5.5/6.2	H3D6213FNLC	
	Ø5.5/6.5	H3D6513FNLC	

Trial Pin for Ultra-wide			
Description	D	Item code	Image/Guide
<ul style="list-style-type: none"> Measures the width and depth of a failed implant site Measures the drilling depth after using the direct drill as the final drill Also serves as a parallel pin 	Ø5.2	HUWFTP52	
	Ø5.5	HUWFTP55	
	Ø6.2	HUWFTP62	
	Ø6.5	HUWFTP65	


Cortical Drill for Ultra-wide			
Description	D/Ø	Item code	Image
<ul style="list-style-type: none"> Trims cortical bone in hard bone cases (for ultra-wide type implants) Drill specifically designed for ultra-wide implant's unique diameter Drilling recommended until the bottom of the marker has been reached 	F6.0	HCD4C60	
	F7.0	HCD4C70	

Drilling Sequence II Type Straight Drill

EKIII | ETIII | SSII


(Length: 10mm)

Ø3.5mm

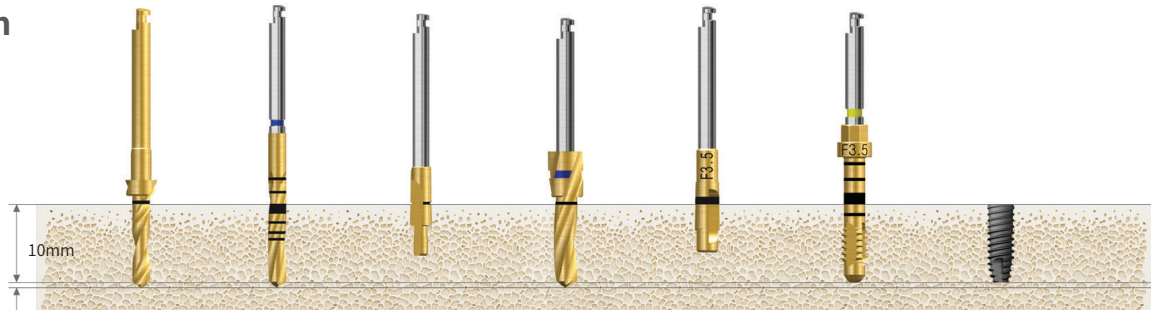


Bone Quality	Ø2.2 Drill	Ø2.7 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	F3.5 Cortical Drill	F3.5 Straight Implant Tap	Ø3.5 Implant
Soft	▶	▶					
Normal	▶		▶	▶			Implant Placement
Hard	▶		▶	▶	▶		
Hard (Option)	▶		▶	▶		▶	

Ø4.0mm

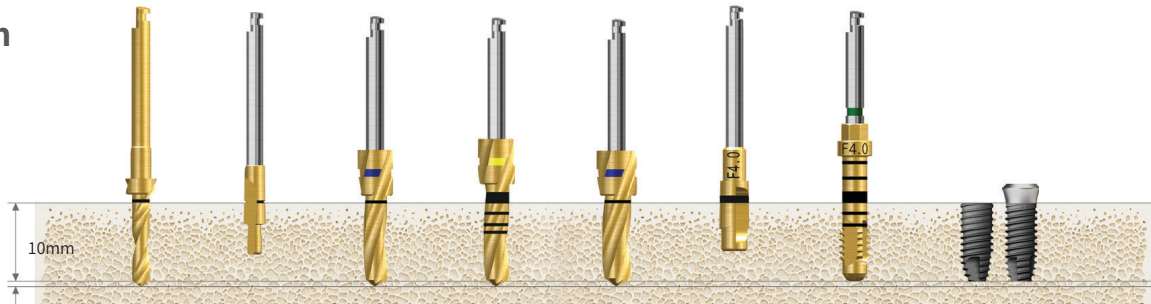

Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.3 Drill	Ø3.8 Drill	F4.0 Cortical Drill	F4.0 Straight Implant Tap	Ø4.0 Implant
Soft	▶	▶	▶	▶				
Normal	▶	▶	▶		▶			Implant Placement
Hard	▶	▶	▶		▶	▶		
Hard (Option)	▶	▶	▶		▶		▶	

Ø4.5mm

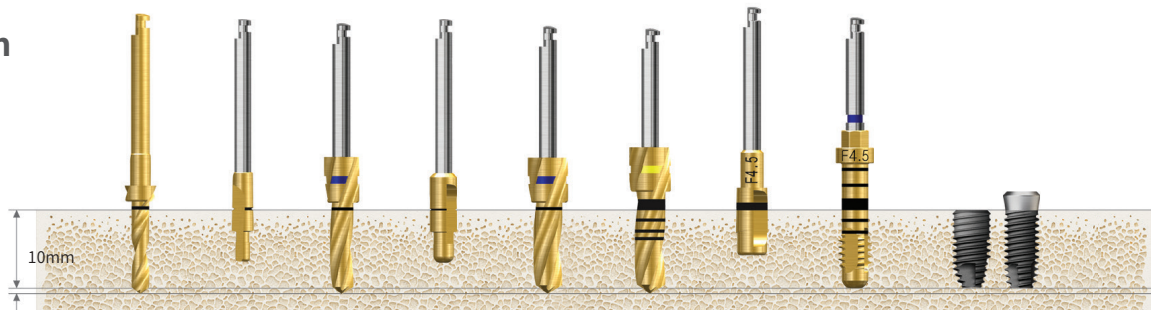


Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.1 Drill	F4.5 Cortical Drill	F4.5 Straight Implant Tap	Ø4.5 Implant
Soft	▶	▶	▶	▶	▶				
Normal	▶	▶	▶	▶	▶	▶			Implant Placement
Hard	▶	▶	▶	▶	▶	▶	▶		
Hard (Option)	▶	▶	▶	▶	▶	▶		▶	

Drilling Sequence III Type Straight Drill

EKIII | ETIII | SSIII


(Length: 10mm)

Ø3.2mm

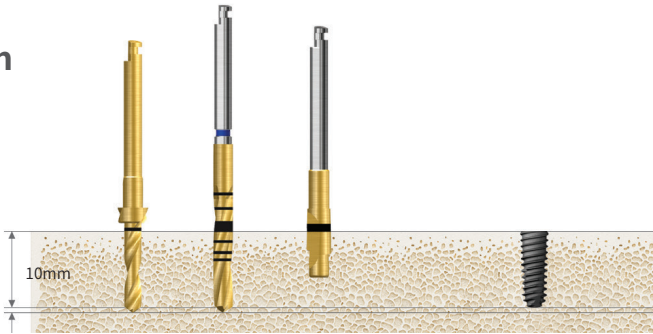

Bone Quality	Ø2.2 Drill	Ø2.7 Drill	F3.0 Cortical Drill 2	Ø3.0 Implant
Soft	▶			Implant Placement
Normal	▶	▶		
Hard	▶	▶	▶	

Ø3.5mm

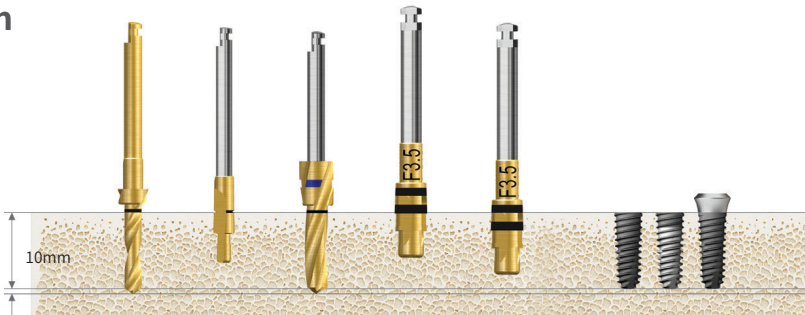


Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	F3.5 Cortical Drill 3	F3.5 Cortical Drill 3	Ø3.5 Implant
Soft	▶	▶	▶			Implant Placement
Normal	▶	▶	▶	▶		
Hard	▶	▶	▶		▶	

Ø4.0mm




Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.3 Drill	F4.0 Cortical Drill 3	F4.0 Cortical Drill 3	Ø4.0 Implant
Soft	▶	▶	▶	▶			Implant Placement
Normal	▶	▶	▶	▶	▶		
Hard	▶	▶	▶	▶		▶	

Ø4.5mm




Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	F4.5 Cortical Drill 3	F4.5 Cortical Drill 3	Ø4.5 Implant
Soft	►	►	►	►	►			Implant Placement
Normal	►	►	►	►	►	►		
Hard	►	►	►	►	►		►	

Ø5.0mm

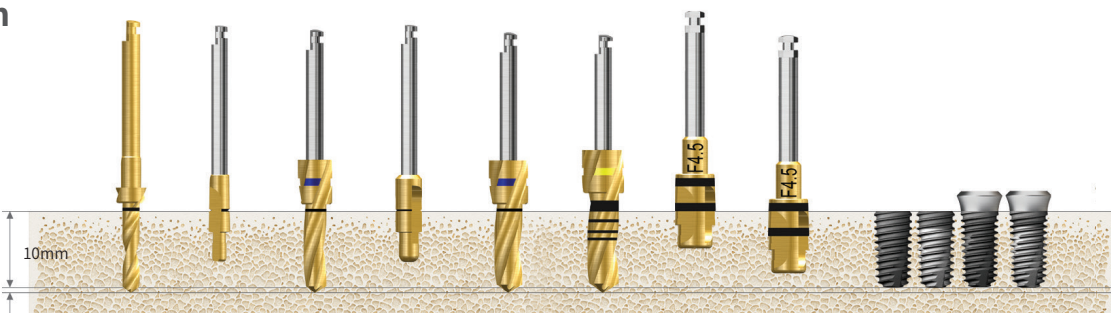

Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.3 Drill	F5.0 Cortical Drill 3	F5.0 Cortical Drill 3	Ø5.0 Implant
Soft	►	►	►	►	►				Implant Placement
Normal	►	►	►	►	►	►	►		
Hard	►	►	►	►	►	►		►	

Ø5.5mm

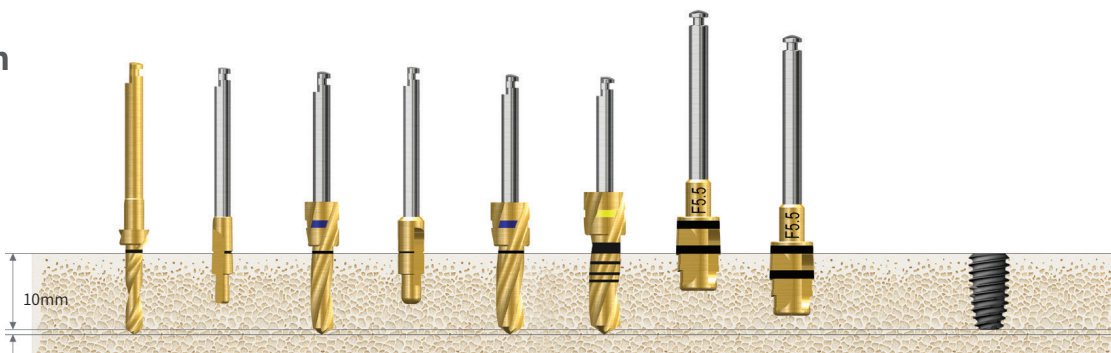

Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.6 Drill	F5.5 Cortical Drill 3	F5.5 Cortical Drill 3	Ø5.5 Implant
Soft	►	►	►	►	►	►			Implant Placement
Normal	►	►	►	►	►	►	►		
Hard	►	►	►	►	►	►		►	

Recommended insertion torque $\leq 40\text{Ncm}$.


ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.

Drilling Sequence IV Type Straight Drill


ETIV

(Length: 10mm)

Ø4.0mm

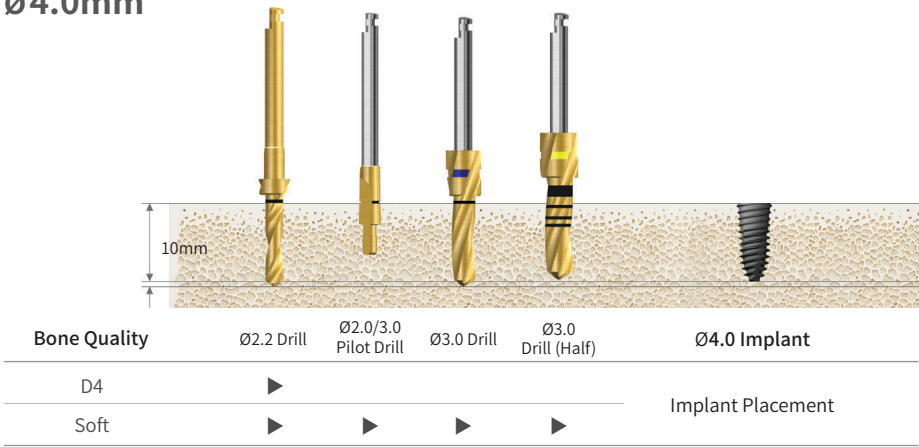

Ø4.5mm

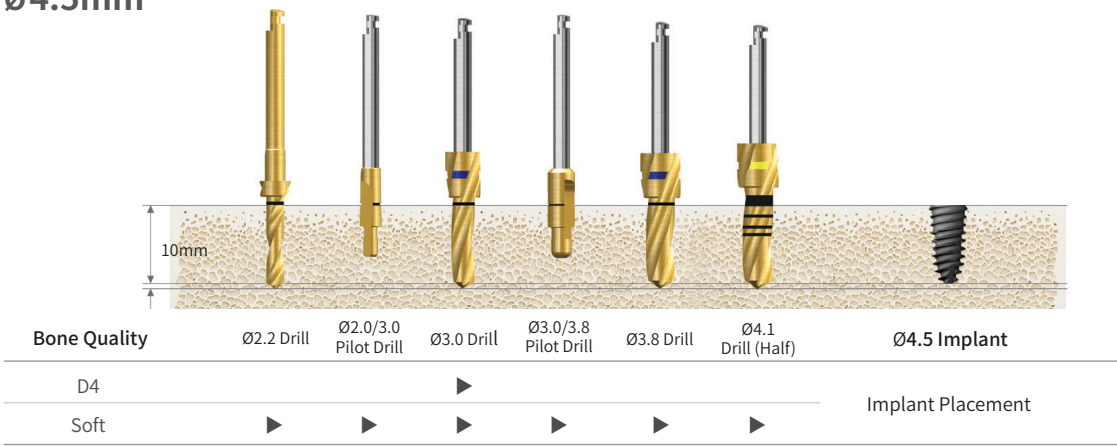

Ø5.0mm



Drilling Sequence Ultra-wide Straight Drill

SSII Ultra-wide

(Length: 10mm)

Ø6.0mm



Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.6 Drill	Ø5.2 Direct Drill	Ø5.5 Direct Drill	F6.0 Cortical Drill	Ø6.0 Implant
Soft	►	►	►	►	►	►	►			
Normal	►	►	►	►	►	►		►		Implant Placement
Hard	►	►	►	►	►	►		►	►	

Ø7.0mm



Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.6 Drill	Ø5.5 Direct Drill	Ø6.2 Direct Drill	Ø6.5 Direct Drill	F7.0 Cortical Drill	Ø7.0 Implant
Soft	►	►	►	►	►	►	►	►			
Normal	►	►	►	►	►	►	►		►		Implant Placement
Hard	►	►	►	►	►	►	►		►	►	


Recommended insertion torque $\leq 40\text{Ncm}$.

ETIV system is designed specifically for the maxillary sinus and soft bone. It is not recommended in the normal bone or hard bone. Recommend reducing the insertion speed to 15rpm or lower, due to the aggressive threads of ETIV


Drilling Sequence **Ultra-wide Straight Drill**

(Length: 10mm)


Ø6.0mm
 Drilling sequence with trephine in the healed mature bone

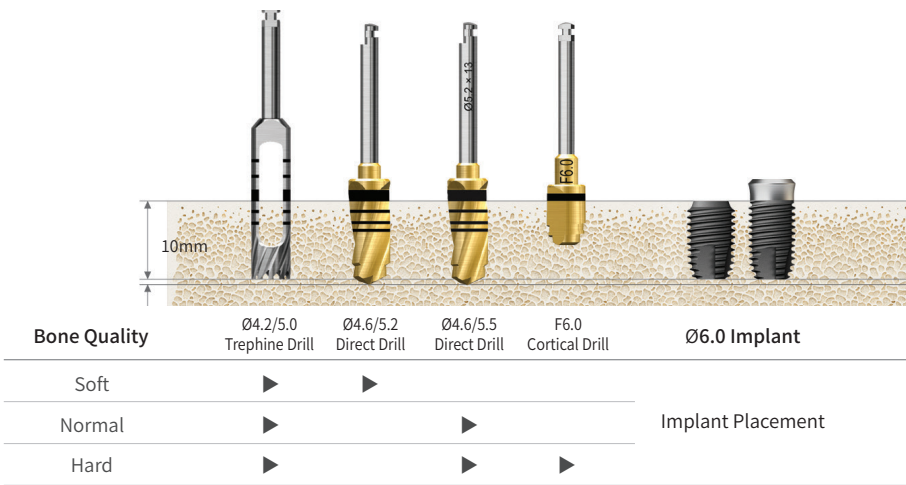

Immediate placement into the extraction socket

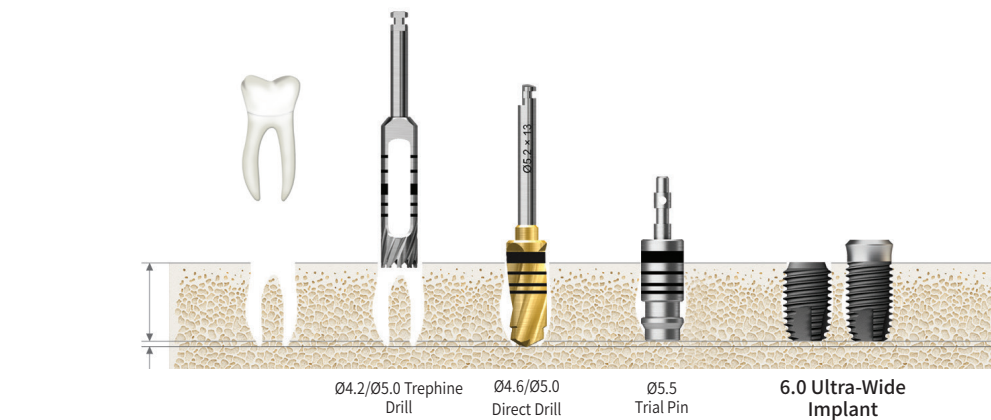

Immediate replacement of the failed implant

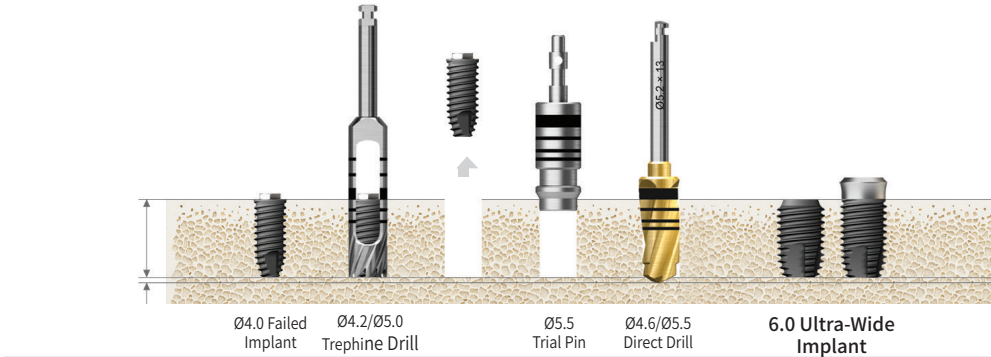


Drilling Sequence Ultra-wide Straight Drill

ETIII Ultra-Wide | SSIII Ultra-wide


(Length: 10mm)

Ø6.0mm

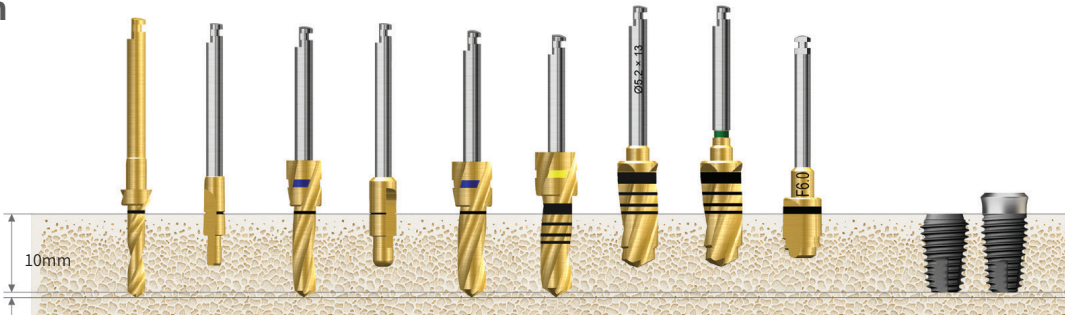

Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.6 Drill	Ø5.2 Direct drill	Ø5.5 Direct drill	F6.0 Cortical Drill	Ø6.0 Implant
Soft	▶	▶	▶	▶	▶	▶	▶			
Normal	▶	▶	▶	▶	▶	▶		▶		Implant Placement
Hard	▶	▶	▶	▶	▶	▶		▶	▶	

Ø7.0mm

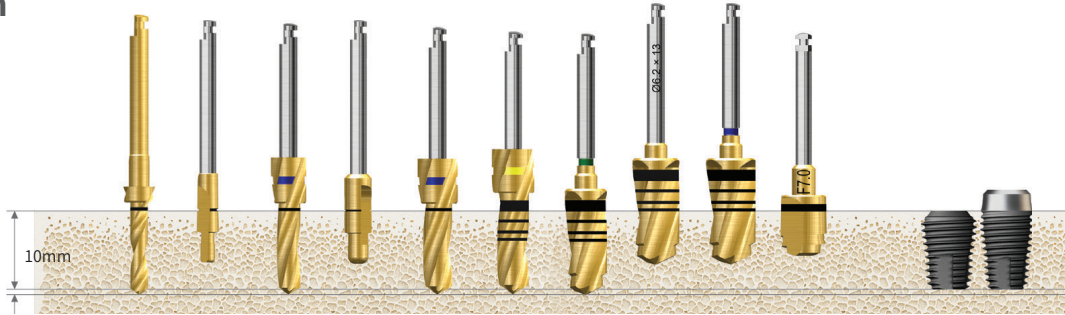

Bone Quality	Ø2.2 Drill	Ø2.0/3.0 Pilot Drill	Ø3.0 Drill	Ø3.0/3.8 Pilot Drill	Ø3.8 Drill	Ø4.6 Drill	Ø5.5 Direct drill	Ø6.2 Direct drill	Ø6.5 Direct drill	F7.0 Cortical Drill	Ø7.0 Implant
Soft	▶	▶	▶	▶	▶	▶	▶	▶			
Normal	▶	▶	▶	▶	▶	▶	▶		▶		Implant Placement
Hard	▶	▶	▶	▶	▶	▶	▶		▶	▶	

Recommended insertion torque $\leq 40\text{Ncm}$.


ET implant insertion depth in normal/hard bone is placed 1mm deeper than the bone level, and the soft bone is placed at the bone level to maintain initial stability.

Drilling Sequence

Ultra-wide Straight Drill

ETIV Ultra-Wide

(Length: 10mm)

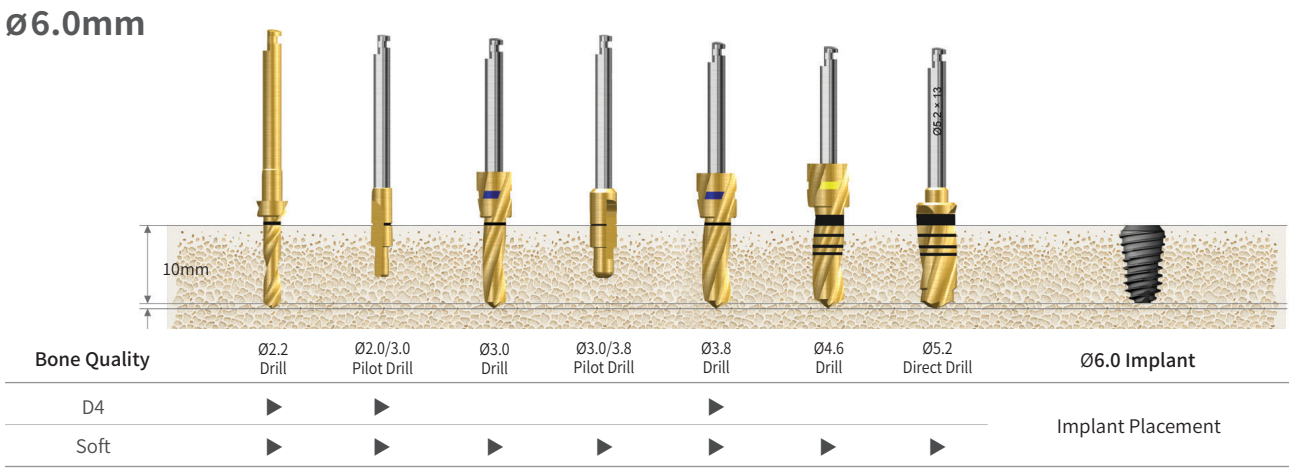


Recommended insertion torque ≤40Ncm







Denture 4U Kit (OD4UK)

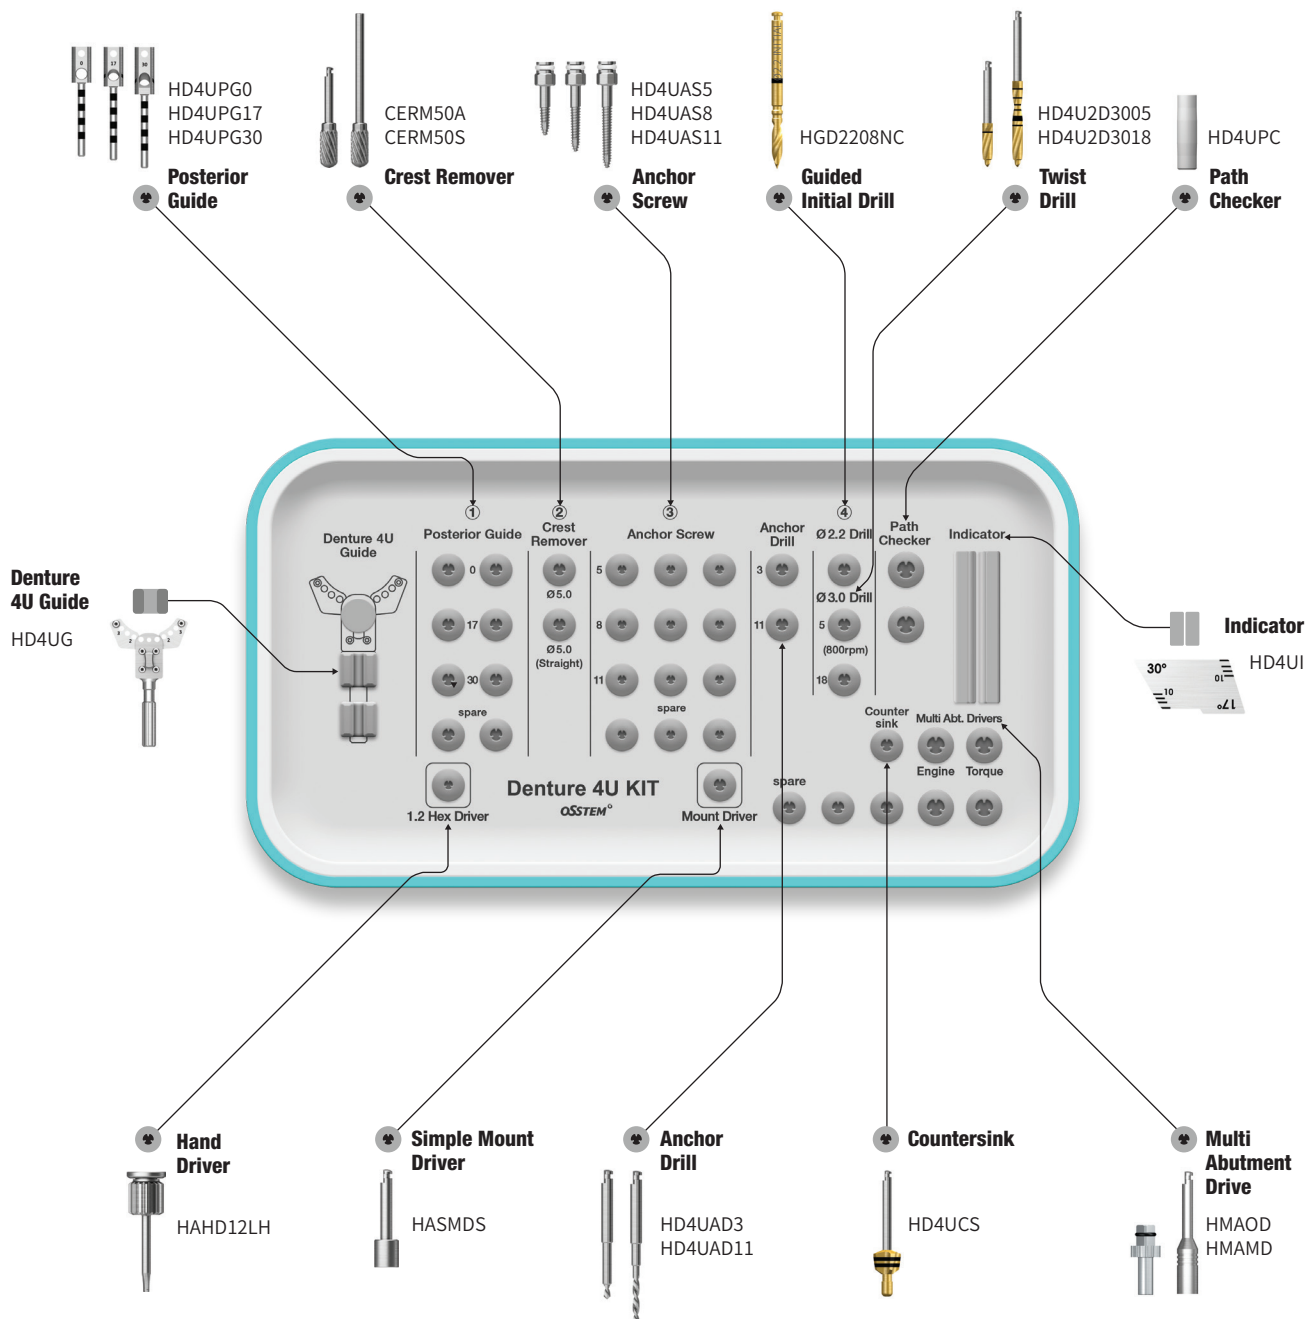

For EKIII ETIII/IV

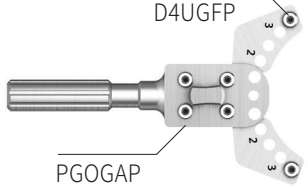




Denture 4U Kit Surgical Instruments



Denture 4U Guide		
Description	Item code	Image
<ul style="list-style-type: none"> Guide for stable and accurate initial and intermediate drilling for Denture 4U Position drill for Ø2.2 in anterior region (tooth no. 2 and 3 positions marked) Anterior guide: drilling positioning for Ø2.2 in anterior region (tooth number 2 and 3 positions marked) Position drill for Ø3,0 drill in posterior region For desired angle, assemble the posterior guide Removable Denture 4U Guide handle 	HD4UG	


Posterior Guide			
Description	Degree	Item code	Image
<ul style="list-style-type: none"> Used by assembling the anterior guide prior to procedure Assembled with the angle marking side shown Adjusting the implant placement position in posterior region and buccolingual inclination angle Selecting the angle of the posterior guide through CT scan recommended prior to procedure Replaceable during procedure Drilling by slowly entering the guide hole, referring to the marking line on the side of the posterior guide hole Drilling depth adjusted by drilling to the bottom marking line in the mesial direction Marking line spacing on the rod: 2mm 	0°	HD4UPG0	
	17°	HD4UPG17	
	30°	HD4UPG30	



Crest Remover				
Description	L	D	Item code	Image
<ul style="list-style-type: none"> Crest remover to in order to set the conditions for Guide Positioning After removing narrowed ridge, mark the implant placement position Recommended speed <ul style="list-style-type: none"> - Angled type: 1,200~1,500rpm - Straight type: 15,000~30,000rpm 	29	Ø5.0	CERM50A	
	45	Ø5.0	CERM50S	


Anchor Screw				
Description	L	D	Item code	Image
<ul style="list-style-type: none"> Used to fix the bone in place by connecting it to the fixed center hole of the Denture 4U Guide and the fixed hole of the posterior guide Fixing the Anchor Screw with the Mount Driver; if the Anchor Screw is not fixed well at this time, it should be drilled first using an Anchor Drill Use first Anchor drill for normal/hard bone Select an appropriate Anchor Screw length according to the degree of the posterior bone retraction Engine stop to prevent Anchor Screw from spinning with no traction when in contact with the guide 	5	Ø1.65	HD4UAS5	
	8	Ø1.65	HD4UAS8	
	11	Ø1.65	HD4UAS11	

Denture 4U Kit Surgical Instruments


Anchor Drill				
Description	L	D	Item code	Image
<ul style="list-style-type: none"> Used to form a hole in normal/hard bone prior to tightening an Anchor Screw Drilling with 3mm drill prior to additional drilling with 11mm drill recommended 	3	Ø1.65	HD4UAD3	
	11	Ø1.65	HD4UAD11	


Guided Initial Drill				
Description	L	D	Item code	Image
<ul style="list-style-type: none"> Used for drilling in anterior region: Ø2.2 drilling into the anterior guide hole of the Denture 4U Guide Drilling by selecting a desired drilling hole of the anterior guide Recommended speed: 800rpm 	5	Ø2.2	HGD2208NC	


Twist Drill				
Description	L	D	Item code	Image
<ul style="list-style-type: none"> Drilling by slowly entering the guide hole, with the angle matched as much as possible, referring to the marking line on the side of the posterior guide hole Drilling depth adjusted by drilling to the bottom marking line in the mesial direction Marking line spacing on the rod: 2mm Recommended speed: 800rpm 	5	Ø1.65	HD4U2D3005	
	18	Ø1.65	HD4U2D3018	

Countersink				
Description			Item code	Image
<ul style="list-style-type: none"> Remove Denture 4U Guide and perform Countersink drilling in order to prevent interference from Taper Drill stoppers and prosthesis. For removing bone interference from the stopper of the Taper Drill Removing bone interference upon mounting a Multi Angled Abutment 			HD4UCS	

Denture 4U Kit Surgical Instruments

Indicator		
Description	Item code	Image
<ul style="list-style-type: none"> Used to check the location of the alveolar nerve, and for the placement direction and length of the implant beforehand for a secure procedure. Perform a full flap surgery in order to spot the mental foramen with naked eye. 	HD4UI	


Path Checker		
Description	Item code	Image
<ul style="list-style-type: none"> Used to check location of the mental foramen by predicting the extended line of the path checker through a panoramic or CT scan For checking the location of the mental foramen without opening a flap completely 	HD4UPC	

Simple Mount Driver			
Description	L	Item code	Image
<ul style="list-style-type: none"> Used for placing an Anchor Screw to stably fix the Denture 4U Guide in place 	Short	HASMDS	

Multi Abutment Machine Driver		
Description	Item code	Image
<ul style="list-style-type: none"> Dedicated Machine Driver for a Multi Abutment 	HMAMD	

Multi Abutment Outer Driver		
Description	Item code	Image
<ul style="list-style-type: none"> Dedicated Torque Driver for a Multi Abutment 	HMAOD	


Prosthetic Simple Kit (HPSK)

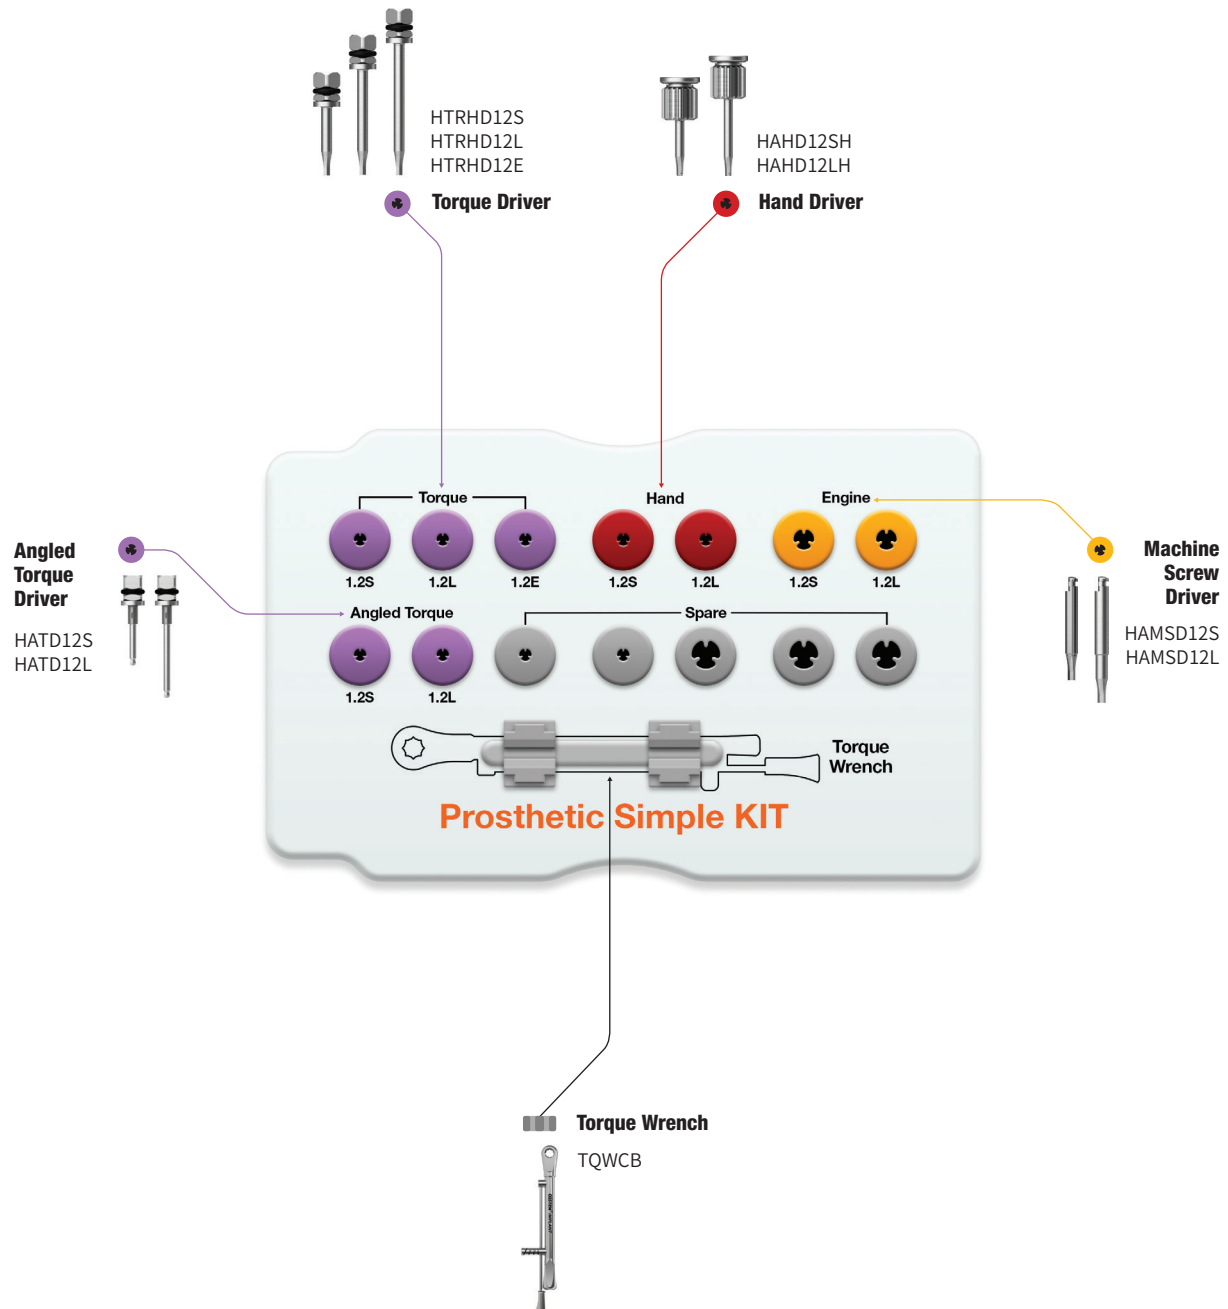


Prosthetic Kit (HPRSTKA)


Top Panel Components


Torque Wrench
TQWCB


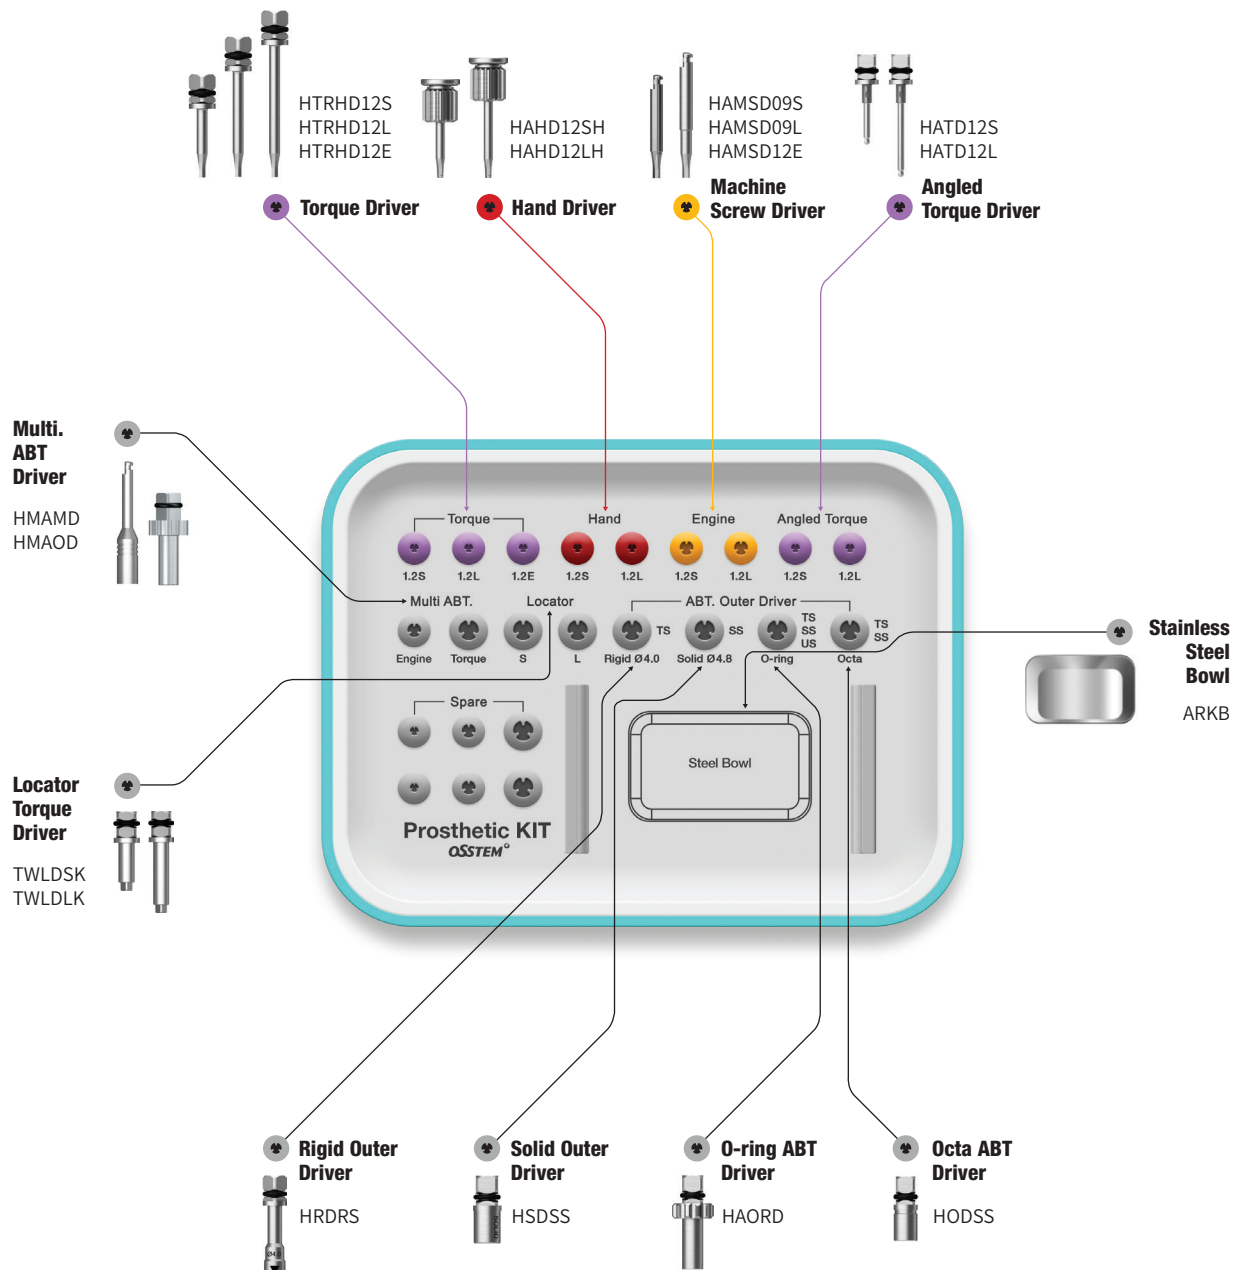




Prosthetic Kit Surgical Kit Instruments





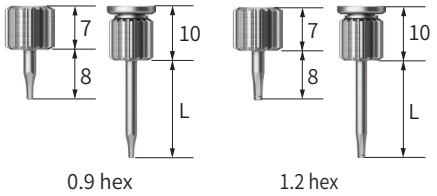
Hand Driver				
Description	L	0.9 Hex	1.2 Hex	Image
<ul style="list-style-type: none"> Manual driver Tip holding function (except internal hex type) Internal hex type length: 11mm 	Ex.Short (8)	HAHD09MSH	HAHD12MSH	
	Short (13)	HAHD09SH	HAHD12SH	
	Middle (15)	-	HAHD12MH	
	Long (18)	HAHD09LH	HAHD12LH	
	Ex.Long (25)	-	HAHD12EH	



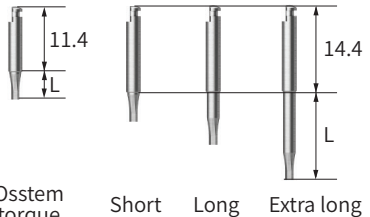


Machine Screw Driver				
Description	L	0.9 Hex	1.2 Hex	Image
<ul style="list-style-type: none"> 1.2 hex driver for engine handpiece Tip holding function (except in internal hex type) Internal hex type length: 8mm 	Osstem Torque (5)	-	-	
	Short (5.6)	HAMSD09S	HAMSD12S	
	Long (11.6)	HAMSD09L	HAMSD12L	
	Ex.Long (17.6)	-	HAMSD12E	
	Application Driver Applied Products (common for hand, machine screw and torque driver)	Cover screw (US mini)	Healing abutment, UCLA, Cemented abutment screw, Mount screw	

Torque Driver					
Description	L	0.5 Slot	0.9 Hex	1.2 Hex	Image
<ul style="list-style-type: none">• Driver for torque wrench• Tip holding function• May bend or break if excessive torque is applied• Damage is possible even at low torque if not fully engaged• Apply vertical pressure when applying torque driver (Do not tilt)• If the tip is bent or stripped, replace immediately	Ex.Short (8)	-	-	HTRHD12MS	
	Short (13)	HTRSD05S	HTRHD09S	HTRHD12S	
	Middle (15)	-	-	HTRHD12M	
	Long (20)	HTRSD05L	HTRHD09L	HTRHD12L	
	Ex.Long (25)	HTRSD05E	-	HTRHD12SE	
					Short Long Extra long

Angled Torque Driver				
Description	L	1.2 Hex	1.2 Hex (Set)	Image
<ul style="list-style-type: none"> Driver for torque wrench No holding function Recommended tightening torque: 30Ncm (excessive torque causes fracture) Do not remove tube to prevent fragmentation when broken Recommended number of use: 10 times Set: 3 per pack 	Short (13)	HATD12S	HATD12S3S	
	Long (20)	HATD12L	HATD12L3S	

Repair Torque Driver			
Description	L	1.2 Hex	Image
<ul style="list-style-type: none"> Reduced diameter of shank compared to the Torque Driver (Ø2.1 → 1.6) The diameter of the screw hole can be minimized during prosthetic repair or SCRP procedures 	Short (13)	HTRHD12SR	
	Long (20)	HTRHD12LR	

Solid Abutment Driver		Regular		Wide	
Description	Type	Short (6)	Long (12)	Short (10)	Long (L)
<ul style="list-style-type: none"> Driver specific for solid abutments Connect to the solid abutment by matching up the groove with the triangular indicator Recommended tightening torque: 30Ncm 	Square	 HSDSS	 HSDSL	 HSD60S	-
	Round	 HSDRS	 HSDRL	-	-

Excellent Solid Abutment Driver		Regular		Wide	
Description	Type	Short (6)	Long (12)	Short (10)	Long (L)
<ul style="list-style-type: none"> Driver for Excellent Solid Abutments Connect to the solid abutment by matching up the groove with the triangular indicator Recommended tightening torque: 30Ncm 	Square	 HESDSS	 HESDSL	 HESD60S	-
	Round	 HESDRS	 HESDRL	-	-

Prosthetic Kit Surgical Kit Instruments


O-ring Abutment Driver		
Description	Item Code	Image
<ul style="list-style-type: none"> Driver for Stud Abutment 	HAORD	



Rigid Outer Driver				
Description	D/Ø (Abutment)	Short (16.5)	Long (21.5)	Image
<ul style="list-style-type: none"> Driver for Rigid Abutments Recommended tightening torque: 30Ncm 	Ø4.0	HRDMS	HORDML	
	Ø4.5	HRD45S	HRD45L	
	Ø5.0	HRDRS	HRDRL	
	Ø6.0	HRDWS	HRDWL	


Octa Abutment Driver			
Description	Type	Short	Long
<ul style="list-style-type: none"> Driver for Octa Abutments Recommended tightening torque: 30Ncm 	Square	12.5 HODSS	18.5 HDSL
	Round	13.4 HDRS	19.4 HDRL



Multi Abutment Machine Driver		
Description	Item Code	Image
<ul style="list-style-type: none"> Machine driver for Multi-Abutments 	HMAMD	

Abutment Holder		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to hold abutments and help deliver them to hard-to-reach sites of the oral cavity 	HOABH	

Multi Abutment Outer Driver		
Description	Item Code	Image
<ul style="list-style-type: none"> Torque driver for Multi-Abutments 	HMAOD	


Locator Abutment Driver			
Description	Type	Item Code	Image
<ul style="list-style-type: none"> Torque driver for Locator Abutments 	Short	TWLDSK	
	Long	TWLDLK	

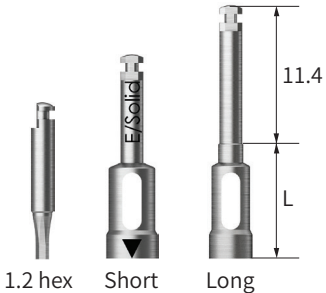
Torque Driver				
Description	Type	Short (10)	Long (15)	Image
<ul style="list-style-type: none"> It may not be fastened or disconnected when connecting a normal handpiece Driver should be used after matching the groove or section of the outer triangle and abutment Solid, excellent solid driver is compatible only with Ø4.8 1.2 hex type L is 5 	1.2 Hex	HTH12S	-	
	Rigid 4.0	HTR40S	HTR40L	
	Rigid 4.5	HTR45S	HTR45L	
	Rigid 5.0	HTR50S	HTR50L	
	Rigid 6.0	HTR60S	HTR60L	
	Solid	HTS48S	HTS48L	
	Excellent Solid	HTE48S	HTE48L	


Path Probe for ET			
Description	Connection	Item Code	Image
<ul style="list-style-type: none"> Tool to check path and measure gingival height after ET implant placement * C = Connection 	Mini	GIPAP-3016A	
	Regular	GIPAP-3516A	



Prosthetic Kit


Surgical Kit Instruments


Torque Connector		
Description	Item Code	Image
<ul style="list-style-type: none"> Tool used convert a square driver connection to a bi-directional connection for the torque wrench 	HRC	


Machine Driver Connector		
Description	Item Code	Image
<ul style="list-style-type: none"> Tool used convert a machine driver into a bi-directional connection for the torque wrench 	HMDC	

Driver Handle		
Description	Item Code	Image
<ul style="list-style-type: none"> Connects to the Torque Driver 	HTIDHC	

Finishing Reamer Set		
Description	Item Code	Image
<ul style="list-style-type: none"> Tool used to remove the excess cast after plastic coping is set <p>Reamer user guide</p> <ol style="list-style-type: none"> 1. Select a reamer tip that is the same size as Abutment size and connect it to the burn-out cylinder 2. Firmly grasp the casting body and rotate the Reamer Bite with consistent force 3. Ream the body until it is clean and free of the excess casting 	HFRSC	

Reamer Bite		
Description	Item Code	Image
<ul style="list-style-type: none"> Tool used to remove the excess cast after plastic coping is set 	HFRBC	

Reamer Tip for Rigid Abutment			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Tool used to remove the excess cast after plastic coping is set 	Ø 4.0	HGSRFRT400	
	Ø 4.5	HGSRFRT450	
	Ø 5.0	HGSRFRT500	
	Ø 6.0	HGSRFRT600	

Reamer Tip for Solid, Excellent Solid Abutment				
Description	Platform	Solid	Ex. Solid	Image
<ul style="list-style-type: none"> Tool used to remove the excess cast after plastic coping is set For both solid Ø6.0 and excellent solid Ø4.8 P = Platform 	Regular Ø4.8	HFRTS480	HF RTE480	
	Wide Ø6.0	HFRTS600	HF RTE600	

EIR Kit Easy Implant Removal Kit (HSFRK)

※ EIR (EK) Kit: **HSFRK**

For

EKIII


ETIII/IV

SSII/III

Ultra-Wide

Top panel components

Implant Wrench
HFRDFE

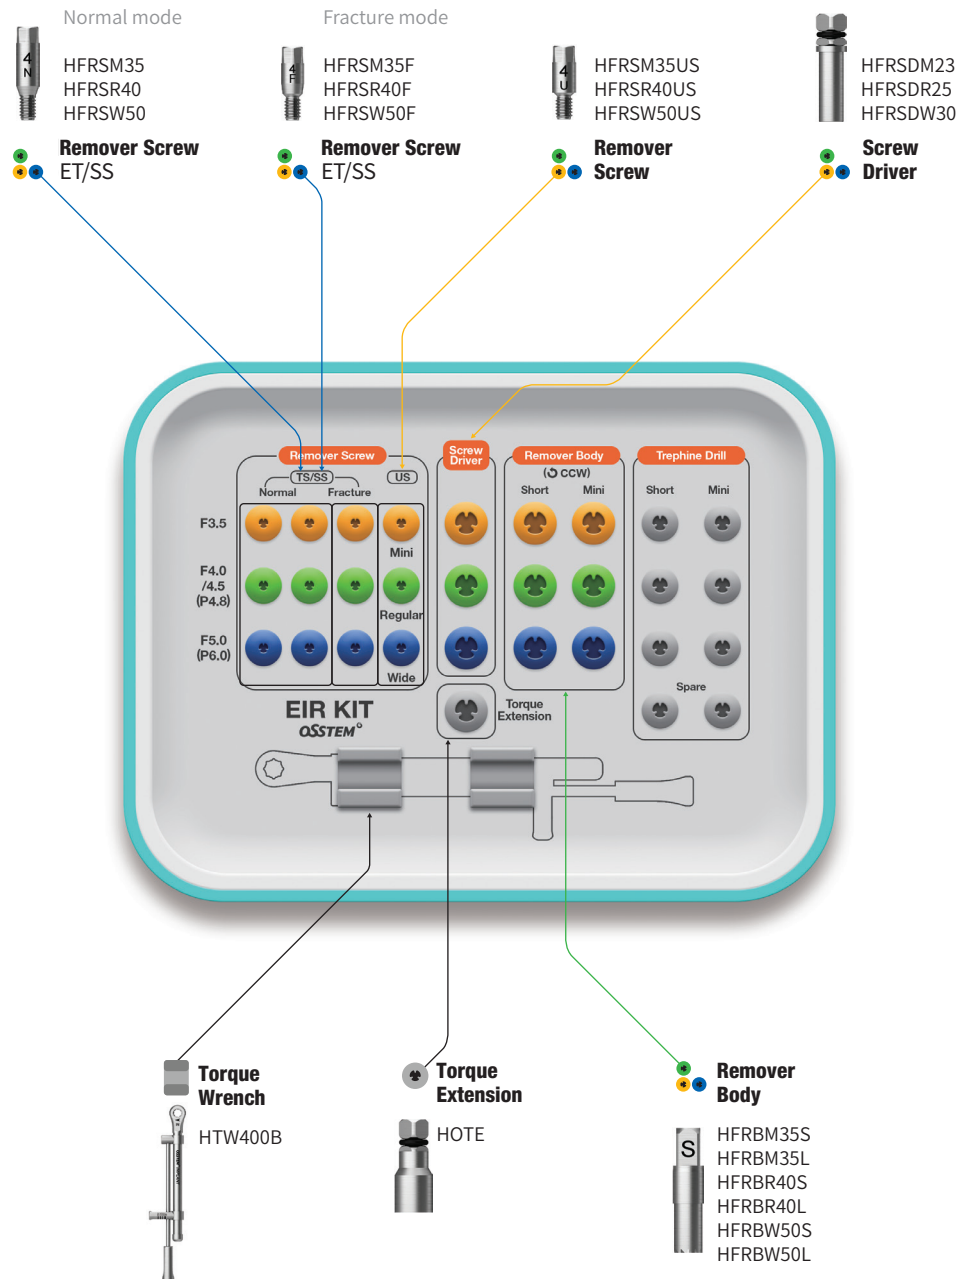

EIR Full Kit Easy Implant Removal Full Kit (HSFRFK_US)



For Nobel Biocare Active/Replace / Straumann Bone Level / Astra Osseo Speed TX
3i Full OSSEOTITE Tapered Certain / Zimmer Tapered / BioHorizons® Internal

Lower panel components


Implant Wrench
HFRDFE



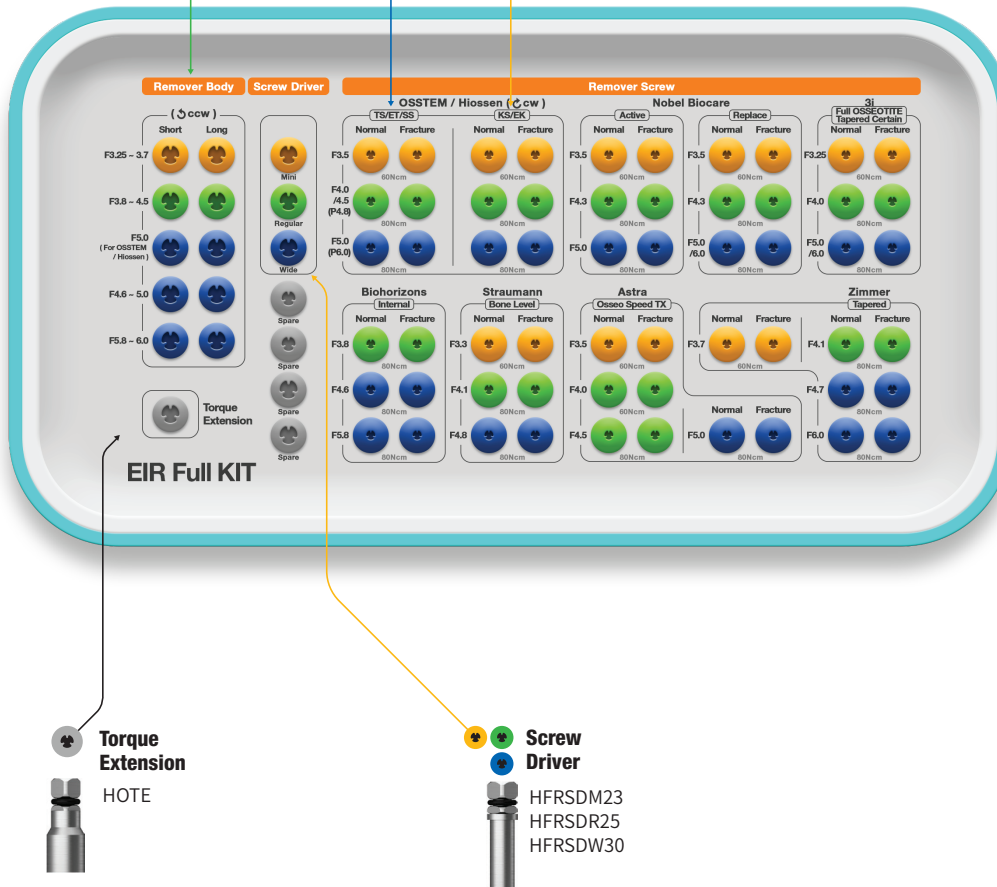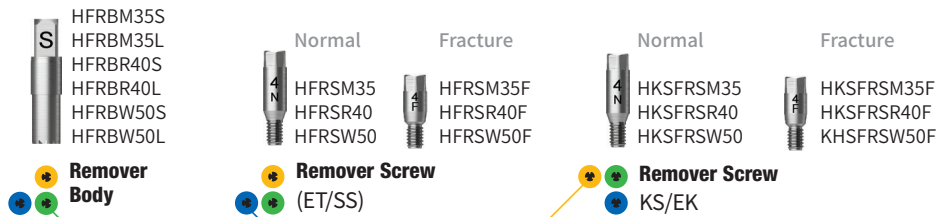

Torque Wrench
HTW400B





EIR Full Kit Surgical Kit Instruments


Remover Screw					
Description			Image		
<ul style="list-style-type: none">When securely fastened to the implant, it serves as a supporting structure for the Remover BodyUse the proper type that matches the diameter of the implant to be removed (ET/SS/US, normal/fracture)Fracture type is specifically for removing a fractured implantRecommended tightening torque: regular/wide 100Ncm, mini 80Ncm ※ Disposable; do not reuse					
Osstem					
Type	Mode	Mini Ø3.5	Regular Ø4.0~4.5/P4.8	Wide Ø5.0/P6.0	
ET/SS	Normal Fracture	HFRSM35 HFRSM35F	HFRSR40 HFRSR40F	HFRSW50 HFRSW50F	
EK	Normal Fracture	HKSFRSM35 HKSFRSM35F	HKSFRSR40 HKSFRSR40F	HKSFRSW50 HKSFRSW50F	
Nobel Biocare					
Type	Mode	Mini Ø3.5	Regular Ø4.3	Wide Ø5.0/6.0	
Active	Normal Fracture	HFRSMNA35 HFRSMNA35F	HFRSR40 HFRSR40F	HFRSW50 HFRSW50F	
Replace	Normal Fracture	HFRSMNR35 HFRSMNR35F	HFRSR40 HFRSR40F	HFRSW50 HFRSW50F	
Straumann					
Type	Mode	Mini Ø3.3	Regular Ø4.1	Wide Ø4.8	
Bone Level	Normal Fracture	HFRSMS33 HFRSMS33F	HFRSRS41 HFRSRS41F	HFRSWS48 HFRSWS48F	
3i					
Type	Mode	Mini Ø3.25	Regular Ø4.0	Wide Ø5.0/6.0	
Full Osseotite Tapered Certain	Normal Fracture	HFRSMS33 HFRSMS33F	HFRSRI40 HFRSRI40F	HFRSWI50 HFRSWI50F	
Biohorizons					
Type	Mode	Mini Ø3.8	Regular Ø4.6	Wide Ø5.8	
Internal	Normal Fracture	HFRSRZ41 HFRSRZ41F	HFRSWZ47 HFRSWB46F	HFRSWZ60 HFRSWB46F	
Astra					
Type	Mode	Mini Ø3.5	Regular Ø4.0	Regular Ø4.5	Wide Ø5.0
Osseo Speed TX	Normal Fracture	HFRSMNA35 HFRSMNA35F	HFRSRA40 HFRSRA40F	HFRSR40 HFRSR40F	HFRSW50 HFRSW50F
Zimmer					
Type	Mode	Mini Ø3.7	Regular Ø4.1	Wide Ø4.7	Ultra-Wide Ø6.0
Tapered	Normal Fracture	HFRSMZ37 HFRSMZ37F	HFRSRZ41 HFRSRZ41F	HFRSWZ47 HFRSWZ47F	HFRSWZ60 HFRSWZ47F

Screw Driver			
Description	F	Item Code	Image
<ul style="list-style-type: none"> Connects and fastens the Remover Screw to the implant Recommended tightening torque: regular/wide 100Ncm, mini 80Ncm 	Mini	HFRSDM23	
	Regular	HFRSDR25	
	Wide	HFRSDW30	

Remover Body				
Description	F	Short	Long	Image
<ul style="list-style-type: none"> Connects to the Remover Screw to apply torque to remove the implant Select the correct type that matches the diameter of the implant to be removed <p>※ Disposable; do not reuse</p>	Mini	HFRBM35S	HFRBM35L	
	Regular	HFRBR40S	HFRBR40L	
	Wide	HFRBW50S	HFRBW50L	
		HFRBW57S	HFRBW57L	
	Ultra-Wide	HFRBUW60S	HFRBUW60L	

Torque Extension		
Description	Item Code	Image
<ul style="list-style-type: none"> Extends the length of the screw driver and remover body (by 10mm) 	HOTE	

Torque Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> Tightens Screw Driver and removes the implant using the Remover Body Applies up to 400Ncm of torque (markers at 80/100/200/300/400Ncm) Torque by pulling the bar back until it reaches the desired torque value marking Clean and sterilize for storage 	HTW400B	

Implant Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> Wrench used to separate the implant from the Remover Body 	HFRDFE	

ESR Kit Easy Screw Removal Kit (HESRK)

※ ESR (EK) Kit: HKESRK


For

EKIII

ETIII/IV

SSII/III


Ultra-Wide

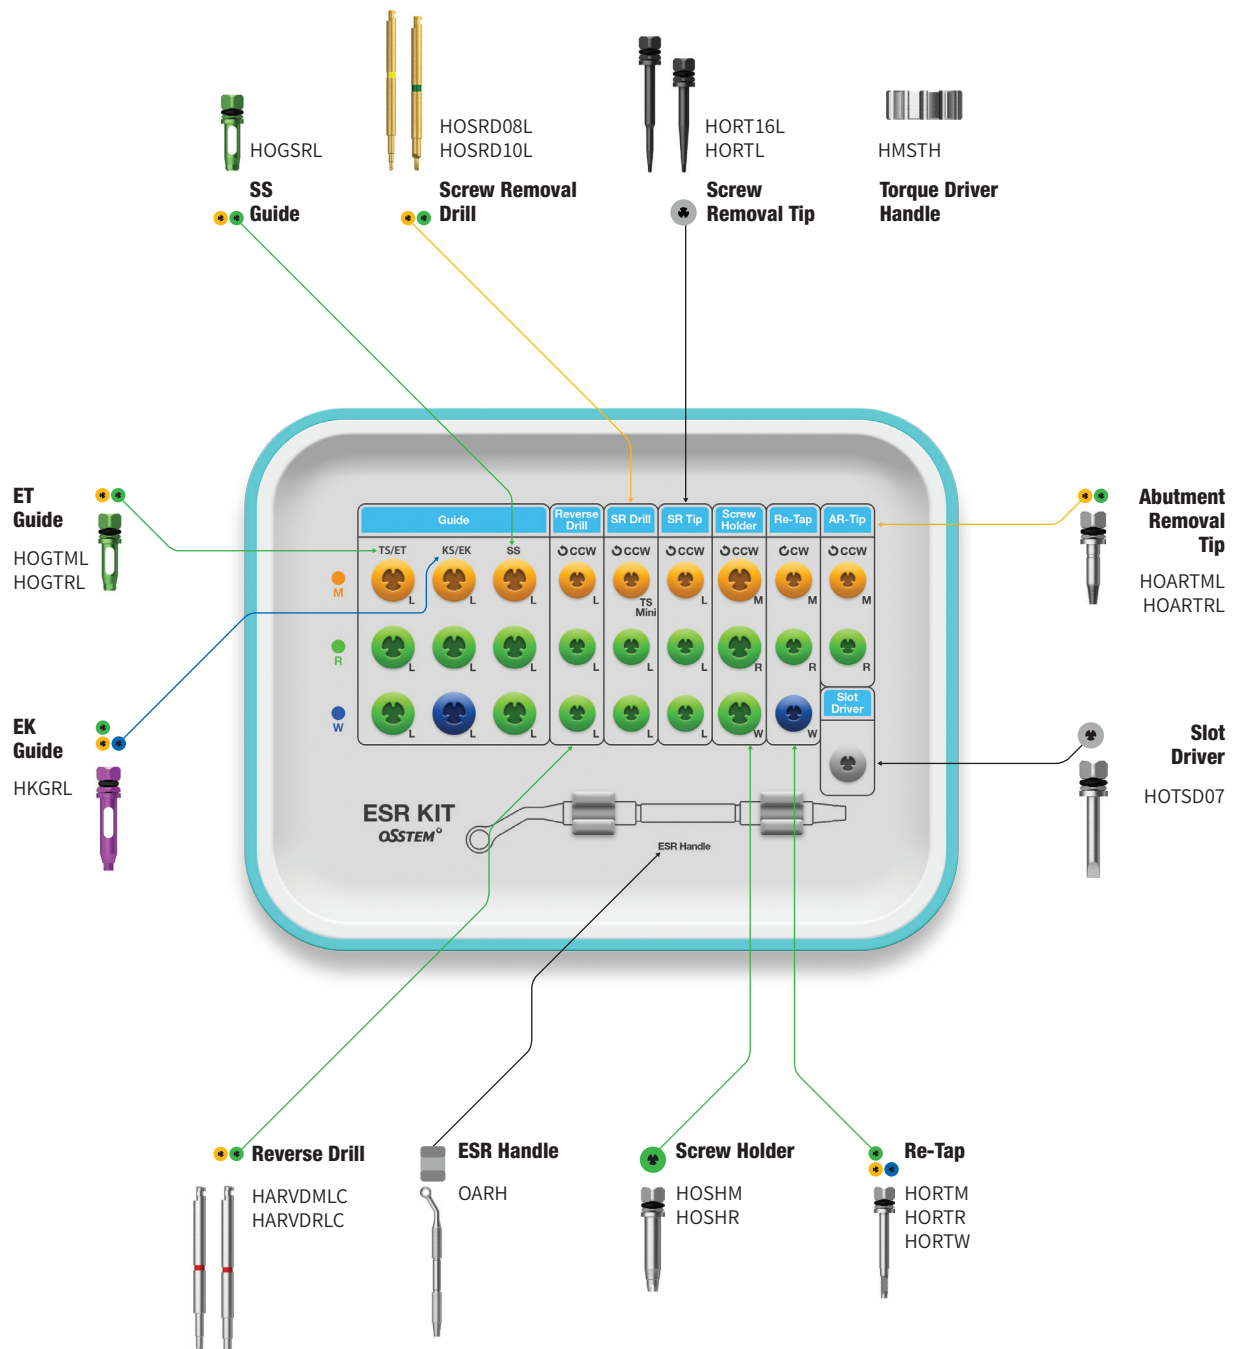







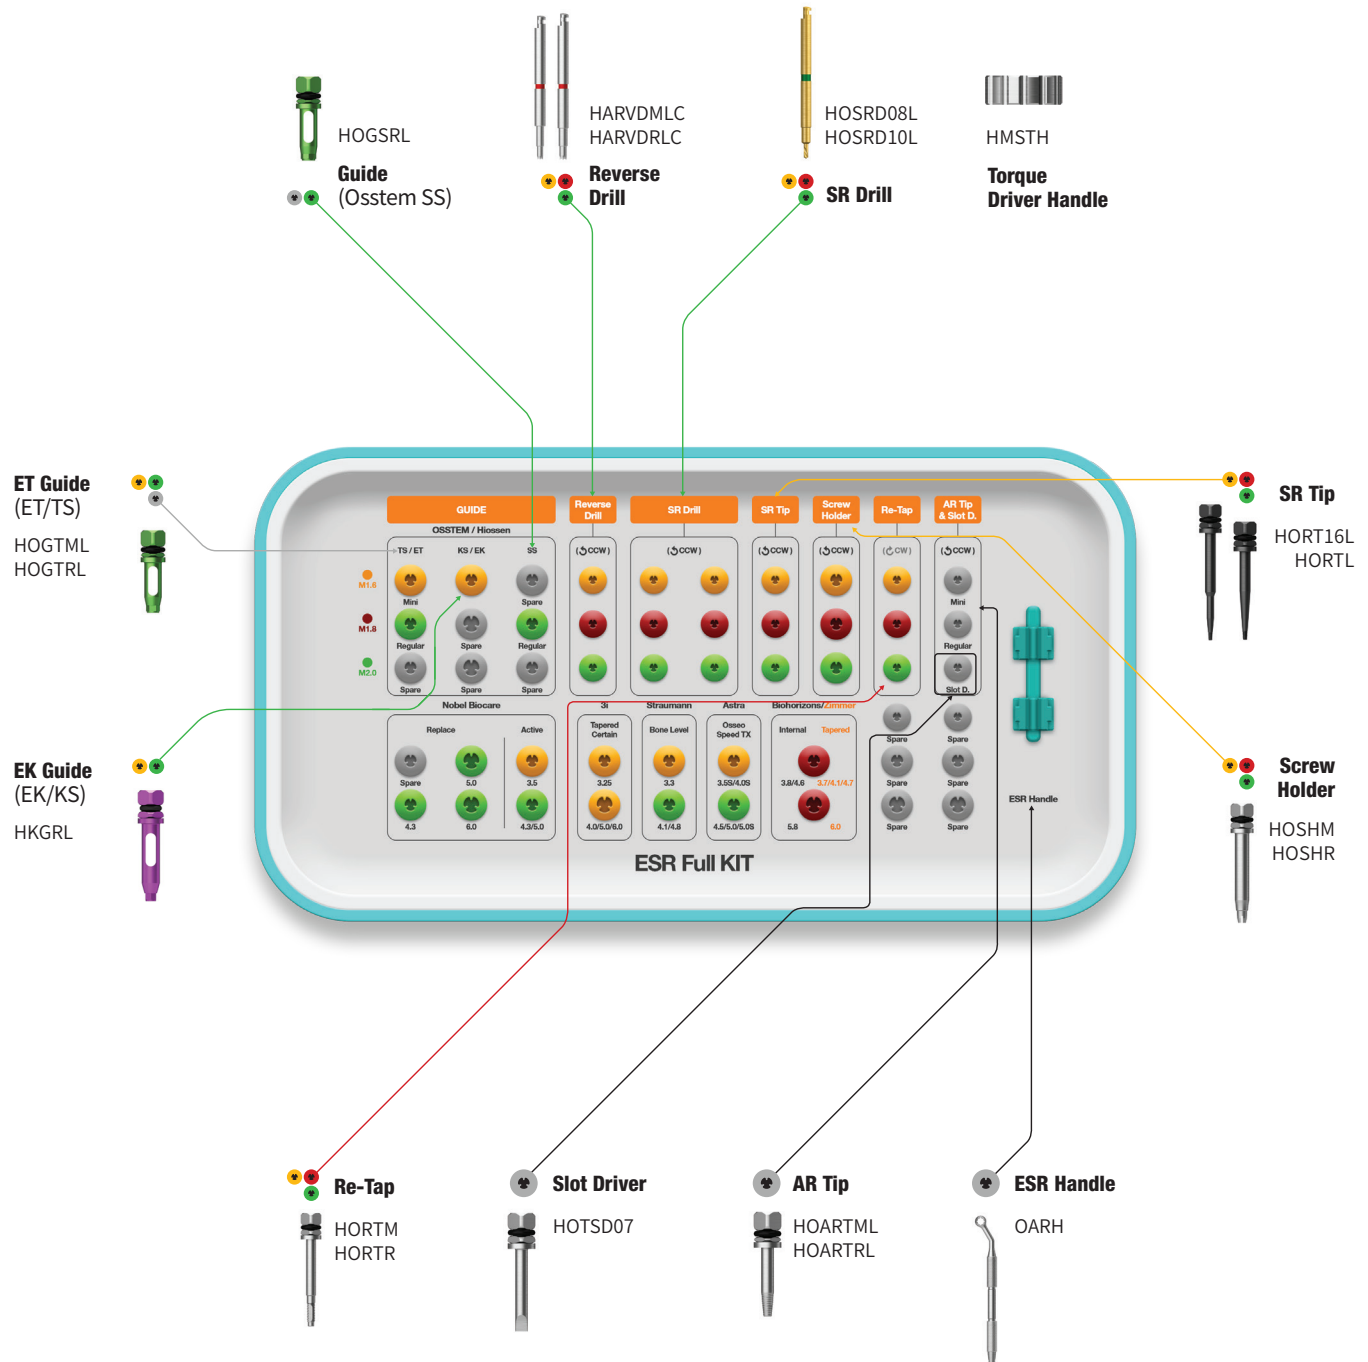

ESR Full Kit Easy Screw Removal Full Kit (HESRFK_US)





For


Nobel Biocare Active/Replace / Straumann Bone Level / Astra Osseo Speed TX
3i Full OSSEOTITE Tapered Certain / 3i Tapered / BioHorizons® Internal




ESR Full Kit Surgical Kit Instruments

Guide							
Description							
<ul style="list-style-type: none">• Connected to the implant to center and prevent shaking of the reverse driver, SR drill and retap• Choose spec of guide according to implant type and diameter (6 overseas companies' internal and submerged type products)• Short or long used according to intermaxillary distance• Used in combination with the ESR handle• *C = Connection/the number of use: 10 times							
Osstem							
Type	Length	C	Mini	Regular	Wide	Image	
ET(TS)	Short		HGTMS	HOGTRS	-		
	Long		HOGTML	HOGTRL	-		
EK(KS)	Short		-	HKGRL	-		
	Long		-		-		
SS	Short		-	HGSRS	HGSRS		
	Long		-	HOGSRL	HOGSRL		
Nobel Biocare							
Type	Length	F	Ø3.5	Ø4.3	Ø5.0	Ø6.0	Image
Active	Short		HGNA01S	HGNA02S	HGNA02S	-	
	Long		HGNA01L	HGNA02L	HGNA02L	-	
Replace	Short		-	HGNR02S	HGNR03S	HGNR04S	
	Long		-	HGNR02L	HGNR03L	HGNR04L	
Type	Length	F	Ø3.3	Ø3.75	Ø4.0	Ø5.0	Image
MKIII	Short		HGUMS	HGURS	HGURS	HGUWS	
	Long		HOGUML	HOGURL	HOGURL	HOGUWL	
Straumann							
Type	Length	F	NC (3.3)	RC (4.1)	RC (4.8)		Image
Bone Level	Short		HGSB01S	HGSB02S	HGSB02S		
	Long		HGSB01L	HGSB02L	HGSB02L		
Type	Length	F	RN (3.3 / 4.1 / 4.8)		WN (4.8)		Image
Roxolid SLActive	Short		HGSTRS		HGSTRS		
	Long		HGSTRL		HGSTRL		
Astra							
Type	Length	F	Small (3.5 S / 4.0 S)		Large (4.5 / 5.0 / 5.0S)		Image
Osseo Speed TX	Short		HGA001S		HGA002S		
	Long		HGA001L		HGA002L		
Zimvie (Zimmer)							
Type	Length	F	Green (3.7 / 4.1 / 4.7)		Green (6.0)		Image
Tapered	Short		HGZB01S		HGZB02S		
	Long		HGZB01L		HGZB02L		



BioHorizons					
Type	Length	F /	Yellow / Green	Blue	Image
Internal (Tapered Bone Level)	Short		HGZB01S	HGZB02S	
	Long		HGZB01L	HGZB02L	
Type	Length	F /	Ø3.5	Ø4.0 / 5.0 / 6.0	
External	Short		HGUMS	HGURS	
	Long		HOGUML	HOGURL	
3i					
Type	Length	F /	3.25	4.0 / 5.0 / 6.0	Image
Full Osseotite Tapered Certain	Short		HGIF01S	HGIF02S	
	Long		HGIF01L	HGIF02L	
Full Osseotite Tapered	Short		-	HGURS	
	Long		-	HOGURL	




Reverse Drill				
Description	Type	Short	Long	Image
<ul style="list-style-type: none"> Used to remove a fractured screw To be used in conjunction with the guide If the red marking of the reverse driver is visible on the guide, remove the fractured screw using a screw holder Direction of rotation: Counterclockwise Recommended number of usage: 10 times 	M1.6	-	HARVDMCL	
	M1.8	HARVDRSC	HARVDRLC	
	M2.0	HARVDRSC	HARVDRLC	




Screw Removal Drill (SR Drill)				
Description	Type	Short	Long	Image
<ul style="list-style-type: none"> Used to create a hole in the fractured screw Make sure to connect the guide, irrigate and suction to remove any debris Available in long and short lengths for different intermaxillary distances Drill until the colored marking on the drill is no longer visible through the guide Recommended speed: 1,200~1,500 rpm (counterclockwise) Recommended number of uses: 5 times Connect the guide before use/Do not apply excessive vertical force/Do not clean with hydrogen peroxide 	M1.6	HSRD08S	HOSRD08L	
	M1.8	HSRD09S	HSRD09L	
	M2.0	HSRD10S	HOSRD10L	




Torque Driver Handle		
Description	Item Code	Image
<ul style="list-style-type: none"> Manual handle for SR Tip, AR Tip, screw holder 	HMSTH	


ESR Full Kit Surgical Kit Instruments



Reverse Driver				
Description	F	Short	Long	Image
<ul style="list-style-type: none"> Reverse Driver Used to remove a fractured screw To be used in conjunction with the guide Insert until the red band is in the Guide and turn counterclockwise to remove the screw Use manually/Rotate counterclockwise/ Number of usages: 10 times 	Mini	-	HRVDML	
	Regular/ Wide	HRVDRS	HRVDRL	


Screw Removal Tip (SR Tip)				
Description	Type	Short	Long	Image
<ul style="list-style-type: none"> Removes a fractured screw by engaging into the hole created by the Screw Removal Drill Rotation direction: counterclockwise 	M1.6	HRT16S	HORT16L	
	M1.8	HRT18S	HRT18L	
	M2.0	HRTS	HORTL	



Screw Holder			
Description	Type	Item Code	Image
<ul style="list-style-type: none"> Grasps onto a protruding fractured screw to unscrew it Color-coded for easy recognition Rotation direction: counterclockwise 	M1.6	HOSHM	
	M1.8	HSHR18	
	M2.0	HOSHR	

Re-Tap			
Description	Type	Item Code	Image
<ul style="list-style-type: none"> Re-threads the internal connection of a implant Connects to a torque wrench or ratchet wrench to re-thread by hand 	M1.6	HORTM	
	M1.8	HRTR18	
	M2.0	HORTR	


ESR Handle		
Description	Item Code	Image
<ul style="list-style-type: none"> Stabilizes the Guide to the implant 	OARH	

Abutment Removal Tip (AR Tip)					
Description	F	Short	Long	Ex. Long	Image
<ul style="list-style-type: none"> Removes fractured or jammed abutments and mounts from the implant Insert into fractured abutment hole, turn counterclockwise, and rock back and forth to loosen and remove with forceps Mini: it can be used to remove a screw with a stripped hex <ul style="list-style-type: none"> To remove the screw, engage the tip into the stripped hex and rotate counterclockwise 	Mini	HARTMS	HOARTML	HARTMEL	
	Regular	HARTRS	HOARTRL	HARTREL	


Slot Driver		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to unscrew a screw, healing abutment, cover screw, or abutment screw with a stripped hex after creating a slot with a Ø0.8 bur 	HOTSD07	


Transfer Abutment Separate Tool			
Description		Item Code	Image
<ul style="list-style-type: none"> Remove jammed abutment of non-hex type transfer abutment The tip is for mini platform abutments; the next step for regular platform Remove the abutment screw, insert Separate Tool Body into the abutment, tighten clockwise with Driver, and remove the abutment. If there is difficulty separating the abutment, attach a ratchet wrench for extra torque 	Driver	HTASD	
	Body	HTASB	
	Set	HTAST	


IM-Cure Kit (HICK)

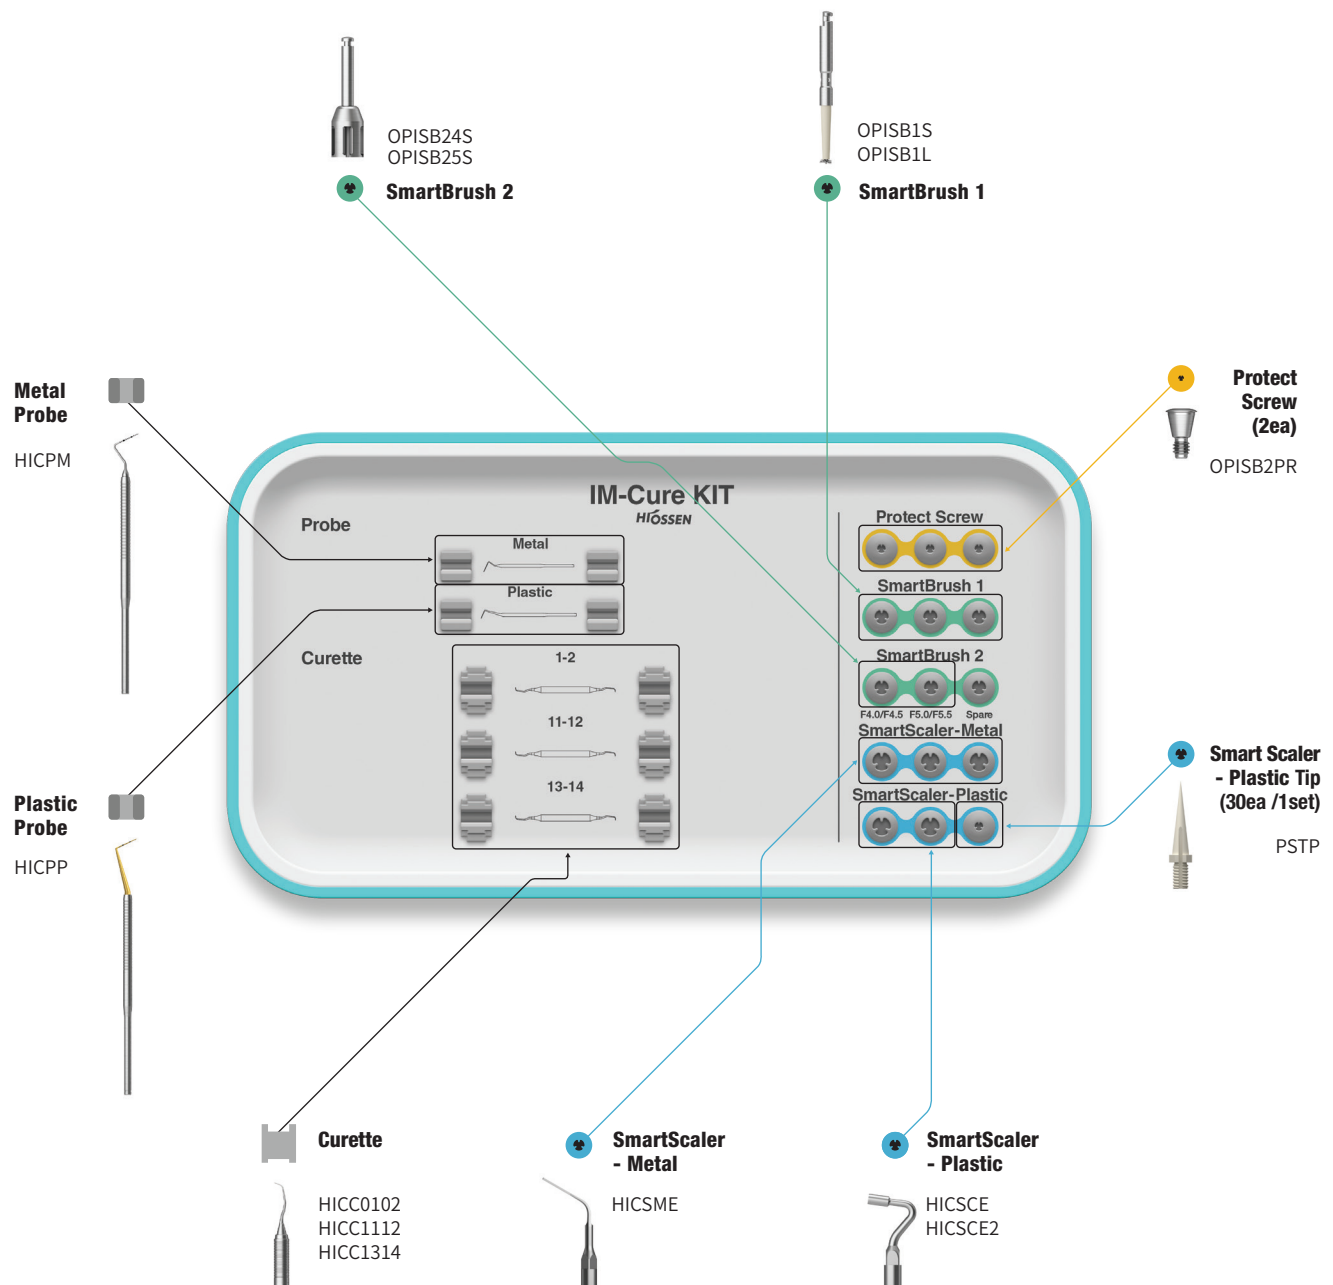


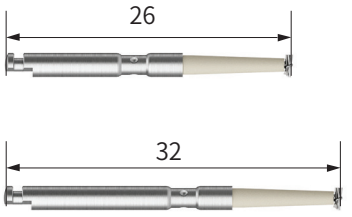
IM-Cure Kit Surgical Kit Instruments

Metal Probe		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to diagnose periodontal disease Measures pocket depth/size Marking lines of 1mm increments 	HICMP	


Plastic Probe		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to diagnose periodontal disease Measures pocket depth/size Marking lines of 1mm increments Plastic material prevents scratches on implant Flexible probe makes it ideal for curved shape of alveolar bone Autoclavable 	HICPP	


Curette			
Description	Type	Item Code	Image
<ul style="list-style-type: none"> Tool to remove granulation tissue firmly attached to a specific area Gracey curette 01-02: used for removal of anterior tissue 11-12: used for removal of ganglion tissue 13-14: used to remove the tissue from the distal part of posterior teeth 	01-02	HICC0102	
	11-12	HICC1112	
	13-14	HICC1314	


Protect Screw			
Description	Type	Item Code	Image
<ul style="list-style-type: none"> Protect the implant's internal connection when using the SmartBrush 1 & 2 Torque Using a 1.2 hex driver, tighten to about 5Ncm 	Mini	OPISB2PM	
	Regular	OPISB2PR	


SmartBrush 1			
Description	Short	Long	Image
<ul style="list-style-type: none"> Bristle designed for effective debridement of the implant surface After removing the patient's prosthesis and abutment, connect the protect screw before using Recommended speed: 1,200~1,500rpm Recommended use time: approximately 1 minute per screw thread (not recommended over 4 minutes) Must use irrigation and suction during polishing <p>※ Disposable. Do not reuse</p>	OPISB1S	OPISB1L	 <p>26</p> <p>32</p>

IM-Cure Kit Surgical Kit Instruments

SmartBrush 2				
Description	D/Ø	Short	Long	Image
<ul style="list-style-type: none"> Debride implant After removing the patient's prosthesis and abutment, connect the protect screw before using Must use irrigation and suction during polishing Recommended speed: 1,200~1,500rpm Recommended use time: 1~2 minutes Excessive use longer than 3 minutes may cause the product to break or bend 	F3.0/F3.5	OPISB23S	OPISB23L	
	F4.0/F4.5	OPISB24S	OPISB24L	
	F5.0/F5.5	OPISB25S	OPISB25L	
	F6.0	OPISB26S	OPISB26L	
	F7.0	OPISB27S	OPISB27L	

SmartScaler - Metal			
Description	Brand	Item Code	Image
<ul style="list-style-type: none"> Used to remove substances such as tartar by connecting it to an ultrasonic scaler Secondary use after using SmartBrush 1 or SmartBrush 2 Easy to bend tip for easy access EMS, KaVo, SATELEC specifications 	EMS KaVo SATELEC	HICSME HICSMK HICSMS	 Bendable

SmartScaler - Plastic				
Description	Brand	125°	100°	Image
<ul style="list-style-type: none"> Used in combination with SmartScaler plastic tip Do not use for removal of debris on the implant surface EMS, KaVo, SATELEC specifications A = Angle 	EMS KaVo SATELEC	HICSCE HICSCK HICSCS	HICSCE2 HICSCK2 HICSCS2	 125° 100°

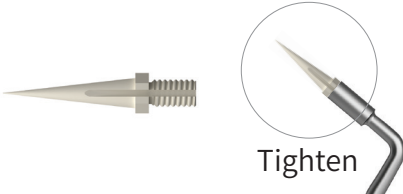SmartScaler Plastic Tip		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to remove substances from abutment or crown by attaching the SmartScaler ※ Do not use to implant surface Packing unit: 30 per set 	PSTP	 Tighten



CAS Kit (HCRSNK)

For **EKIII** **ETIII/IV** **SSII/III** **Ultra-Wide**

Top panel components

Lower panel components

Hydraulic Membrane Lifter Tube
SNMT


Bone Carrier Head
SNBCH30



Bone Carrier
SNBCS35



Bone Condenser
SNBC1114

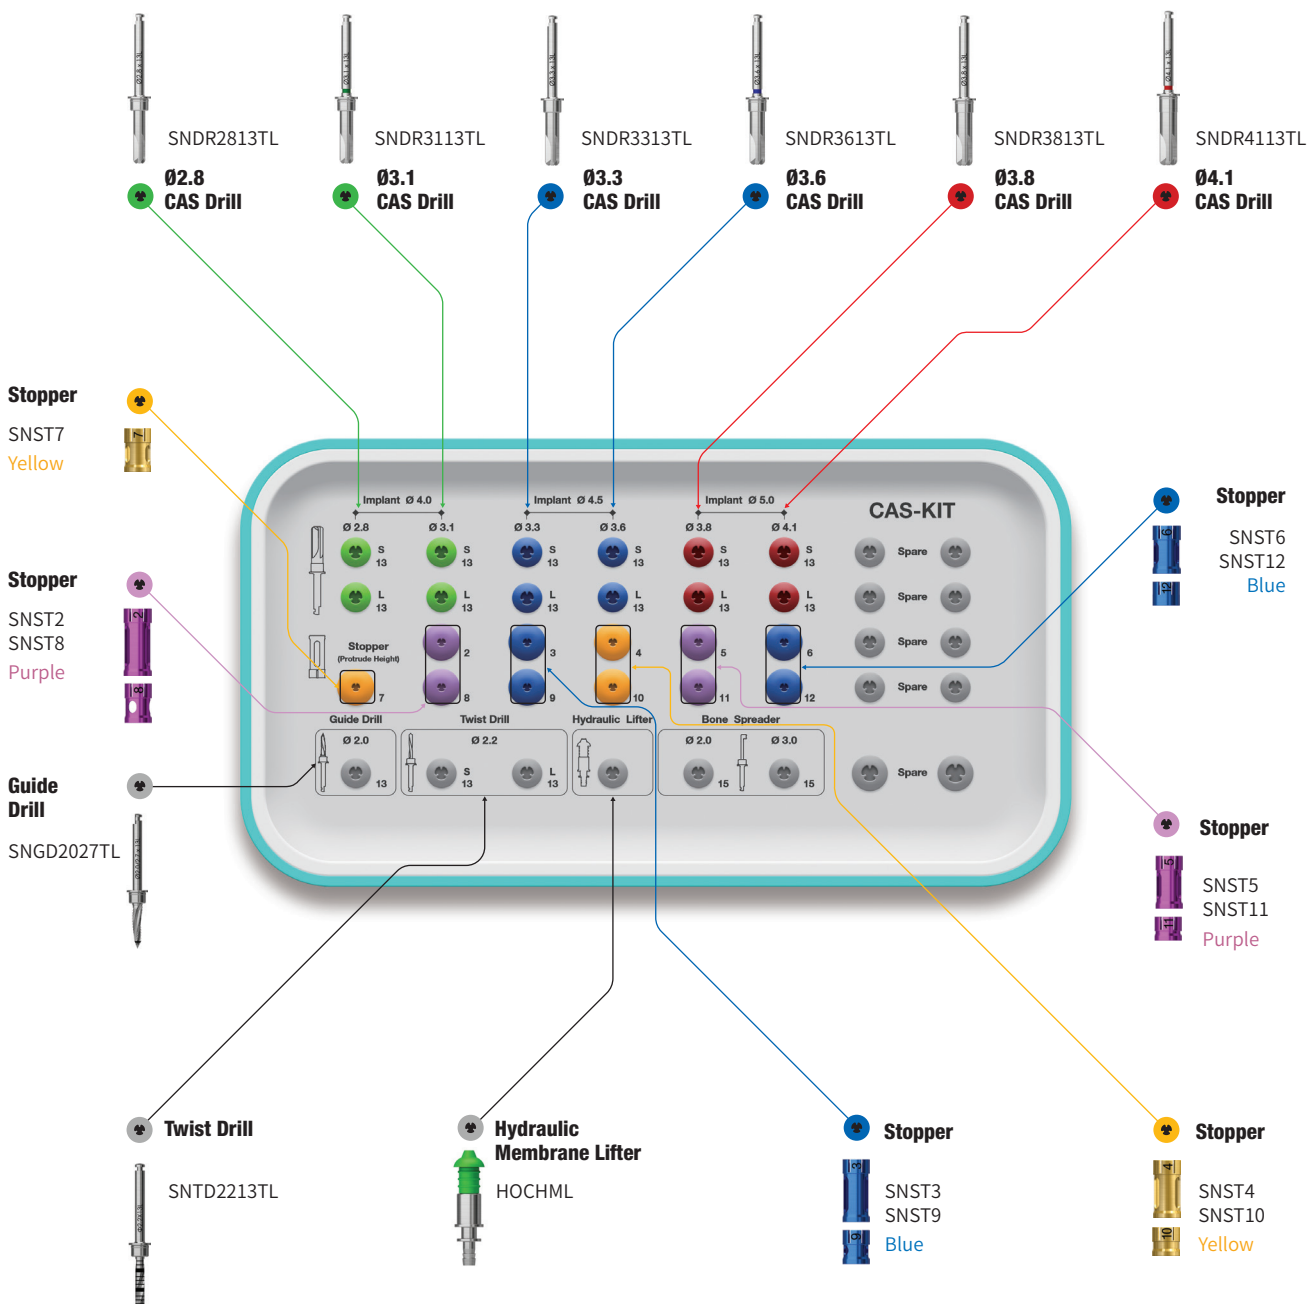

CAS Kit Surgical Kit Instruments

CAS Drill				
Description	D/Ø	Short	Long	Image
<ul style="list-style-type: none"> Specialized drill designed to penetrate the sinus floor without damaging the Schneiderian membrane by forming a conical bone lid Four blade drill design provides superior bone removing capability from low to high speeds, and can collect autogenous bone at low speeds Safely advance to the floor of the sinus using stoppers (1mm increments) Final drill diameter is based on bone density, regardless of the implant type (straight or tapered) Recommended speed: 400~800rpm (For beginner: 400rpm) 	Ø2.8	SNDR2813TS	SNDR2813TL	
	Ø3.1	SNDR3113TS	SNDR3113TL	
	Ø3.3	SNDR3313TS	SNDR3313TL	
	Ø3.6	SNDR3613TS	SNDR3613TL	
	Ø3.8	SNDR3813TS	SNDR3813TL	
	Ø4.1	SNDR4113TS	SNDR4113TL	


Guide Drill			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Drill to mark the implant placement site Side cutting blades can be used to modify the side walls of the extraction socket Line marking 2mm from the apex of drill 	Ø2.0/2.7	SNGD2027TL	



Ø2.2 Twist Drill			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Recommended to under-drill by 1mm below the floor of the sinus Use with stoppers for safe and controlled drilling Apex tip measures an additional 0.6mm 	Ø2.2	SNTD2213TL	


Hydraulic Membrane Lifter Set			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Hydraulic pressure is used to separate and lift the sinus membrane Securely fits Ø2.8~Ø4.1 CAS drilled osteotomies 	Ø2.6/6.0	HOCHML	


Stopper											
<ul style="list-style-type: none"> Laser mark numbers indicates drilling depth Color-coded by length Recommended number of usage: 50 times 											
Length	2	3	4	5	6	7	8	9	10	11	12
Item Code	SNST2	SNST3	SNST4	SNST5	SNST6	SNST7	SNST8	SNST9	SNST10	SNST11	SNST12
Color	Purple	Blue	Yellow	Purple	Blue	Yellow	Purple	Blue	Yellow	Purple	Blue


CAS Kit Surgical Kit Instruments


Bone Carrier		
Description	Item Code	Image
<ul style="list-style-type: none"> Handle for the bone carrier head Connects the bone carrier head and tighten at the opposite end Connects both heads (SNBCH30 or SNBCH35) 	SNBCS35	



Bone Carrier Head			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Cone shaped with an extended tip that reaches the sinus cavity and prevents bone material from spilling out SNBCH30 for Ø3.1/3.3 CAS drilled osteotomy SNBCH35 for Ø3.6/3.8/4.1 CAS drilled osteotomy Fill the reservoir (up to the marker) with bone material in small quantities using the bone condenser. Repeat the process as necessary 	Ø3.1	SNBCH30	
	Ø3.6	SNBCH35	


Bone Condenser		
Description	Item Code	Image
<ul style="list-style-type: none"> Safely pushes bone material through the bone carrier into the sinus cavity SNBCH30: use Ø1.1/SNBCH35: use Ø1.4 	SNBC1114	

Hydraulic Membrane Lifter Tube		
Description	Item Code	Image
<ul style="list-style-type: none"> Tubing to connect the hydraulic membrane lifter to the saline filled syringe 	SNMT	

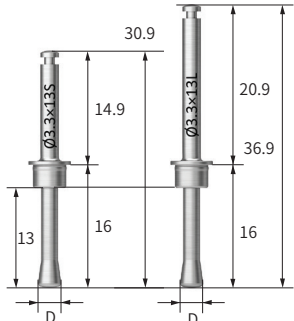
Membrane Lifter				
Description	D/Ø	Short	Long	Image
<ul style="list-style-type: none"> Round shape with no cutting edges for safe membrane lifting Select Membrane Lifter diameter according to the CAS drill diameter used (head diameter: CAS drill diameter -0.2mm) Use CAS stoppers to control length Recommended speed: 30~50rpm (Recommended speed for beginner: 30rpm) Be sure to spray water when using 	Ø2.6	SNML2813TS	SNML2813TL	
	Ø2.9	SNML3113TS	SNML3113TL	
	Ø3.1	SNML3313TS	SNML3313TL	
	Ø3.4	SNML3613TS	SNML3613TL	
	Ø3.6	SNML3813TS	SNML3813TL	
	Ø3.9	SNML4113TS	SNML4113TL	

Depth Gauge		
Description	Item Code	Image
<ul style="list-style-type: none"> Checks for access into the sinus cavity and measures the thickness of residual bone 	SNDG	

Bone Spreader			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Spreads bone graft material in the sinus cavity Used with CAS stoppers Recommended speed: 30rpm or less 	Ø2.0	SNBS2015T	
	Ø3.0	SNBS3015T	

Y-Connector		
Description	Item Code	Image
<ul style="list-style-type: none"> Y-type connecting tool capable of simultaneous hydraulic pressure elevation in two osteotomies 	SNYCT	

LAS Kit (HLRSNK)

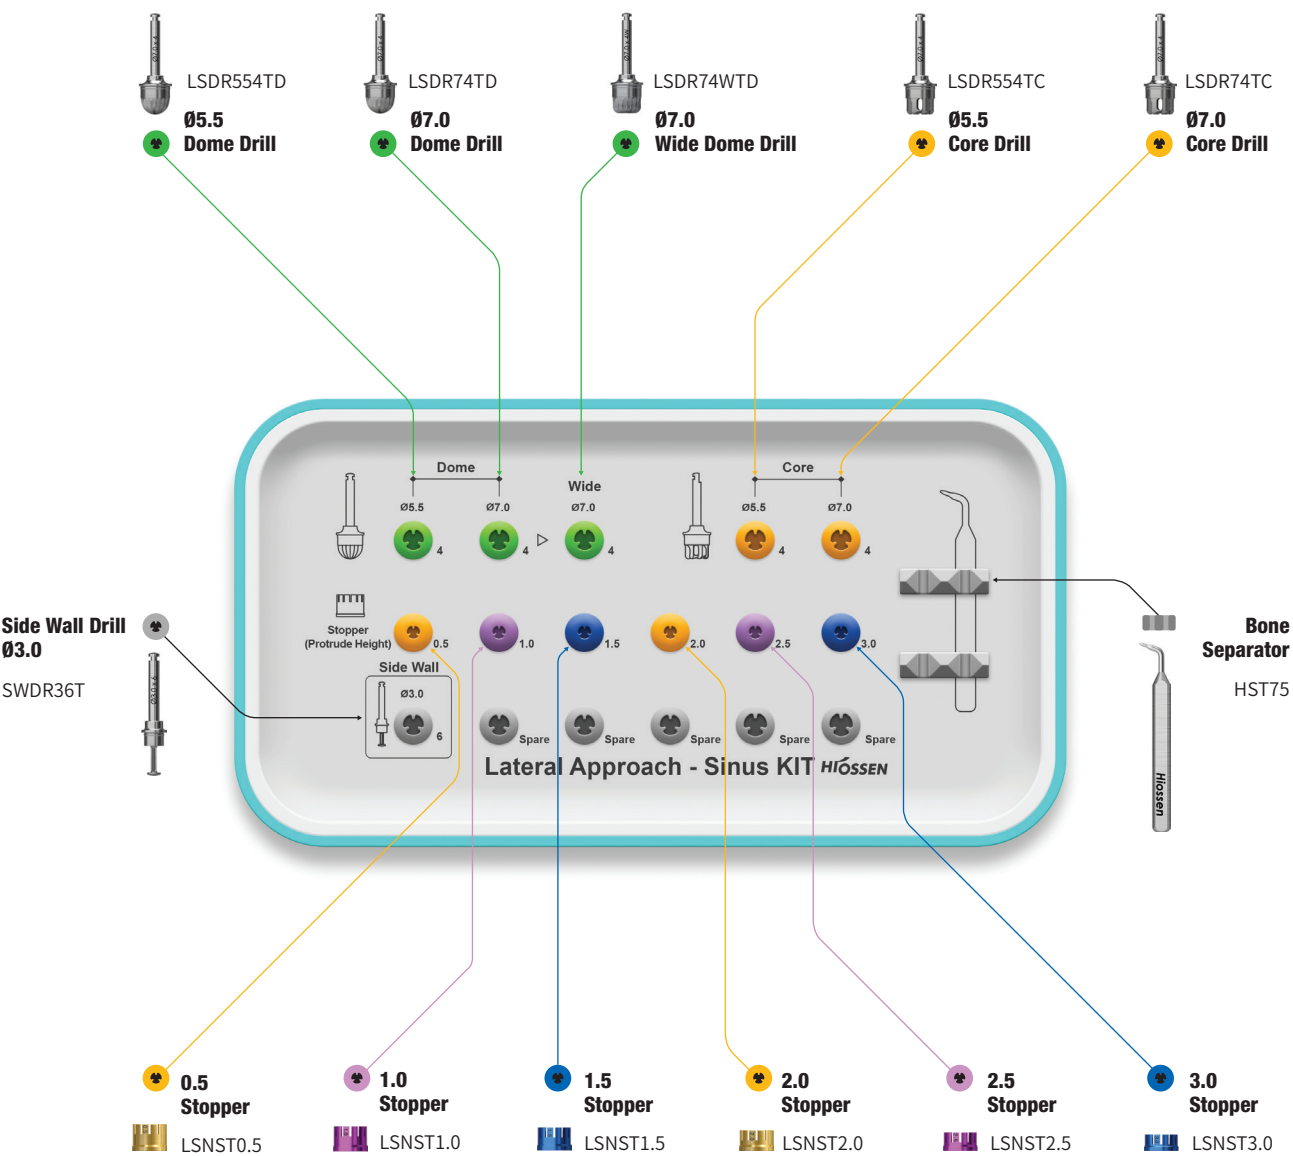

LAS Kit Surgical Kit Instruments

Dome Drill			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Dome Drill Forms a bone window and collects autogenous bone simultaneously Excellent penetration due to the combination of macro and micro cutting edges Stopper system safely controls the penetration depth Recommended speed: 1,200~1,500rpm Excessive drilling may cause damage to the membrane 	Ø5.5 Ø7.0	LSDR554TD LSDR74TD	
	Wide Ø7.0	LSDR74WTD	

Core Drill			
Description	D/Ø	Item Code	Image
<ul style="list-style-type: none"> Creates a bone lid while forming the lateral window Cutting edge design based on the CAS drill, enhancing safety Recommended speed: 1,200~1,500rpm Excessive drilling may cause damage to the membrane 	Ø5.5 Ø7.0	LSDR554TC LSDR74TC	

Side Wall Drill						
Description	Item Code		Image			
<ul style="list-style-type: none"> Enlarges and trims the rough edges of the bone window Cutting blades start 1 mm above the bottom of the drill Recommended speed: 1,500rpm 	SWDR36T					
Height of side cutting blade (mm)	1.0	2.0	3.0	4.0	.05	
CAS Kit stopper (mm)	8.0	9.0	10	11	12	
Side wall Drill + CAS Kit stopper • Stoppers safely control the drilling depth						

Bone Separator		
Description	Item Code	Image
<ul style="list-style-type: none"> Removes the bone lid inside the core drill 	HST75	

Side Wall Drill							
Description	Length	0.5	1.0	1.5	2.0	2.5	3.0
<ul style="list-style-type: none"> Laser marked numbers indicate the drilling depth Color-coded by length Can be used up to 50 times before replacement 							
	Item Code Color	LSNST0.5 Yellow	LSNST1.0 Purple	LSNST1.5 Blue	LSNST2.0 Yellow	LSNST2.5 Purple	LSNST3.0 Blue

ESSET Kit (HESEK)


For EKIII ETIII/IV SSII/III Ultra-Wide

Lower panel components

Torque Wrench
TQWCB



Depth Gauge
ODG

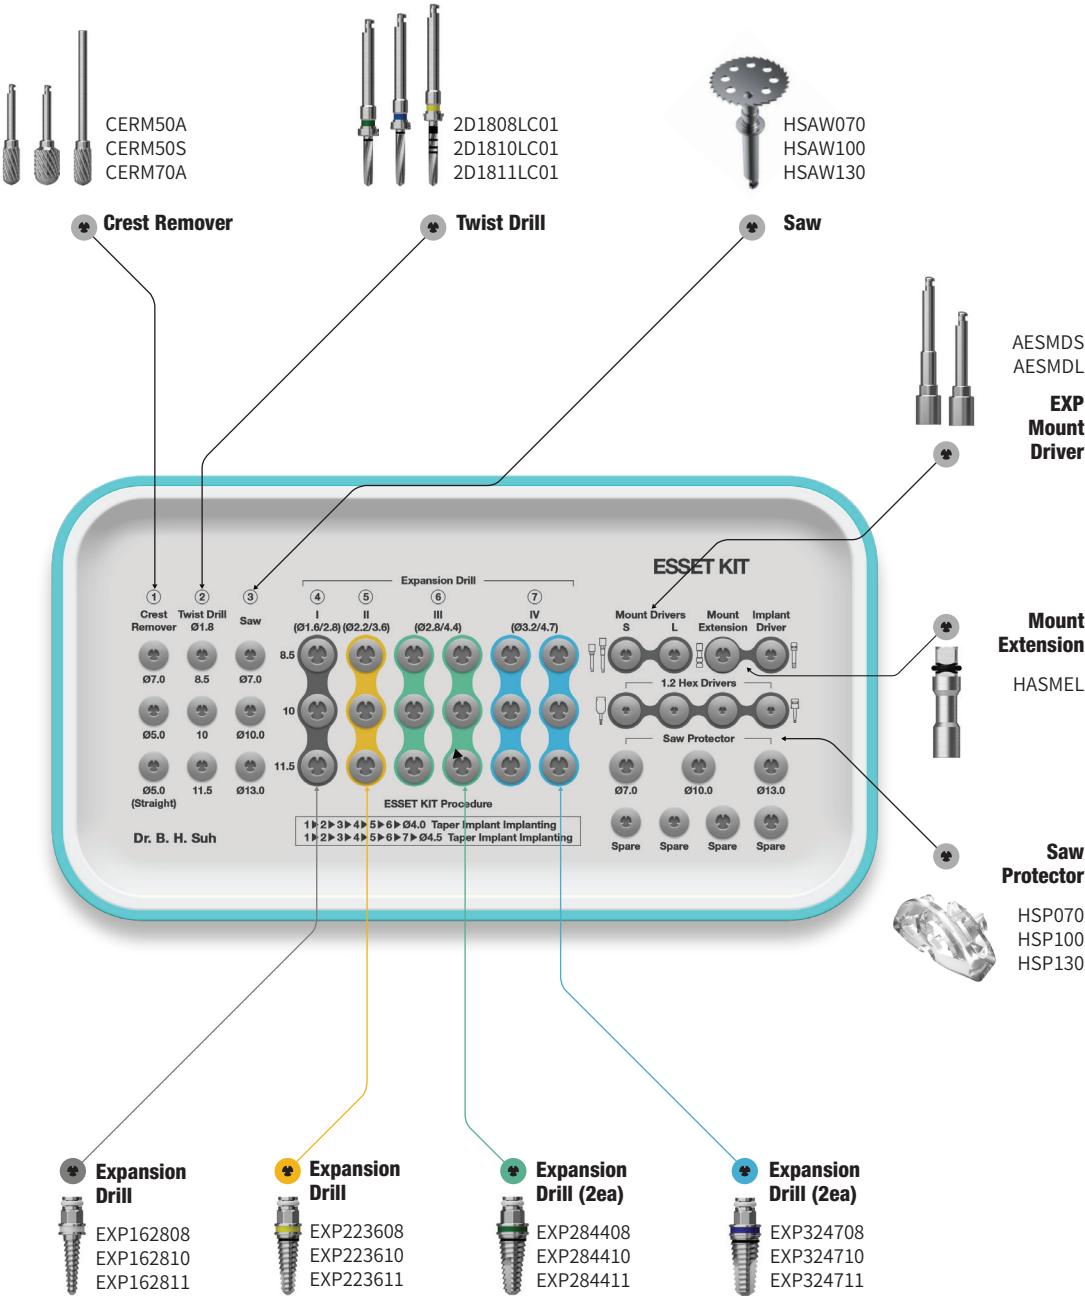

ESSET Kit Surgical Kit Instruments

Crest Remover				
Description	L	Ø5.0	Ø7.0	Image
<ul style="list-style-type: none"> Grinds down narrow alveolar ridge, and creates an indentation for the implant's insertion site Angled type recommended speed: 1,200~1,500rpm Straight type recommended speed: 15,000~30,000rpm 	29	CERM50A	CERM70A	
	45	CERM50S	-	

Twist Drill				
Description	L	TL	Ø1.8	Image
<ul style="list-style-type: none"> Marks the implant's insertion site Controls depth with the built-in stopper Recommended speed: 1,200 ~ 1,500 rpm 	8.5	33	2D1808LC01	
	10	34.5	2D1810LC01	
	11	36	2D1811LC01	

Saw				
Description	T	TL	Item Code	Image
<ul style="list-style-type: none"> For ridge modification and splitting After vertical incision, move from mesial to distal Recommended speed: 1,200 ~ 1,500 rpm Recommended use: 10 times *T = Thickness 	0.3	Ø7.0	HSAW070	
		Ø10	HSAW100	
		Ø13	HSAW130	

Saw Protector			
Description	D	Item Code	Image
<ul style="list-style-type: none"> Semi-circular saw cover protects user when using saws See through protector for maximum procedure visibility 360° rotary saw cover for flexible operation Material: Plastic <p>※ Single use only (Do not reuse)</p>	Ø7.0	HSP070	
	Ø10	HSP100	
	Ø13	HSP130	

ESSET Kit Surgical Kit Instruments

Expansion Drill					
Description	Type	8.5	10	11.5	Image
<ul style="list-style-type: none"> Gradually expands narrow alveolar ridge Use the Expansion Drills in numerical order based on the diameter of the implant F4.0: I → II → III/F4.5: I → II → III → IV Recommended speed: 25~35rpm 	I Ø1.6/2.8	EXP162808	EXP162810	EXP162811	
	II Ø2.2/3.6	EXP223608	EXP223610	EXP223611	
	III Ø2.8/4.4	EXP284408	EXP284410	EXP284411	
	IV Ø3.2/4.7	EXP324708	EXP324710	EXP324711	

Mount Extension		
Description	Item Code	Image
<ul style="list-style-type: none"> Used to apply manual torque when inserting/removing the Expansion Drills 	HASMEL	

EXP Mount Driver			
Description	Length	Item Code	Image
<ul style="list-style-type: none"> Used to inserting/removing the Expansion Drills with a handpiece and engine 	Short (22.1)	AESMDS	
	Long (28.6)	AESMDL	

Torque Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> Use to apply torque to the Expansion Drill 	TQWCB	


Depth Gauge		
Description	Item Code	Image
<ul style="list-style-type: none"> Releases excessive torque when hand piece does not move due to being stuck in bone during expansion drill removal process. Use with an open wrench to turn the hex of the Expansion drill Prevents from over torquing 	ODG	




EM (MS) Kit (HMISLK)

Lower panel components



Depth Gauge
HMDTGG



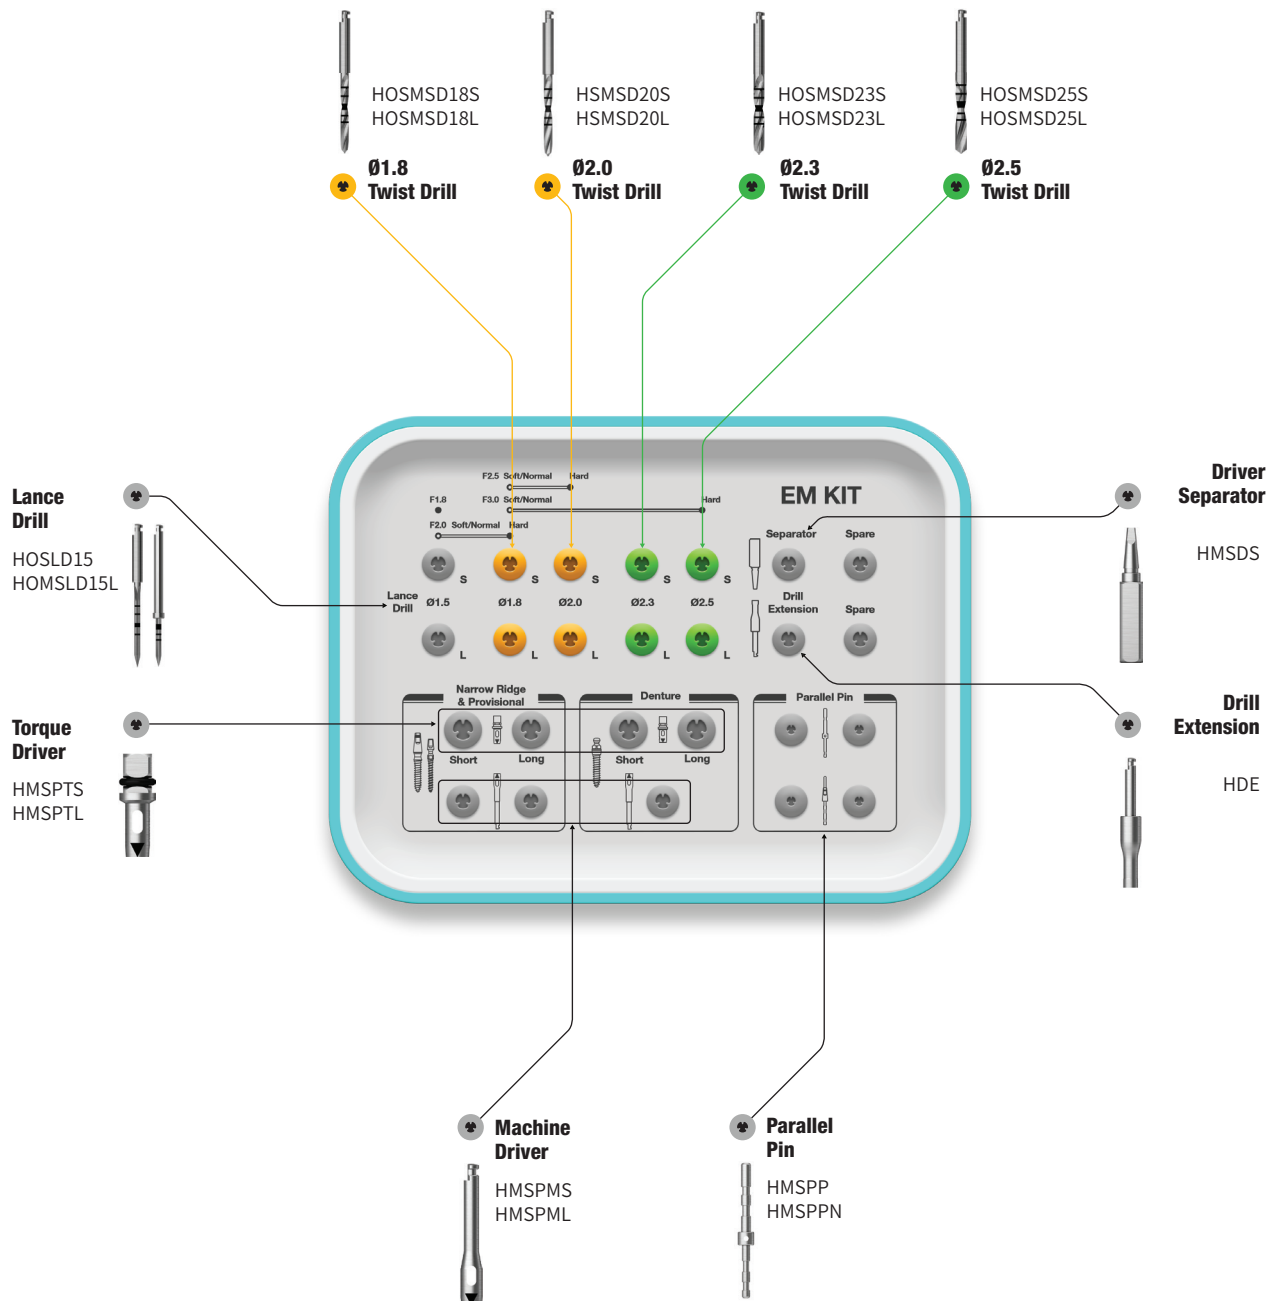

Ratchet Wrench
CITQW-1185A





EM (MS) Kit Surgical Kit Instruments


Drill for EM (MS) Implant							
Description	Length	Ø1.5	Ø1.8	Ø2.0	Ø2.3	Ø2.5	Image
<ul style="list-style-type: none"> Laser markings on drill match implant length specifications (8/10/11.5/13/15 mm) In cortical bone, it is recommended to use the lance drill to drill to the final implant length Long type has a stopper at 13mm 	Short (35)	HOMD1508	-	-	-	-	
	Long (38)	HOMD1510	-	-	-	-	
	Short (33)	-	HOSMSD18S	HSMSD20S	HOSMSD23S	HOSMSD25S	
	Long (31)	-	HOSMSD18L	HSMSD20L	HOSMSD23L	HOSMSD25L	


Driver for Narrow Ridge & Provisional Type				
Description		Length	Ø3.4	Image
<ul style="list-style-type: none"> Driver for EM (MS) implants: narrow ridge & provisional The triangular marking is used in line with the implant 	Torque Driver	Short (16.5) Long (21.5)	HMSPTS HMSPTL	
	Machine Driver	Short (24.4) Long (29.4)	HMSPMS HMSPML	

Driver for Denture Type				
Description		Length	Ø3.8	Image
<ul style="list-style-type: none"> Driver for EM (MS) Implant denture The triangular marking should be aligned with the implant 	Torque Driver	Short (13.5) Long (18.5)	HMSDTS HMSDTL	
	Machine Driver	Long (21.4)	HMSDMS	

Gauge for MS Implant				
Description		Length	Item code	Image
<ul style="list-style-type: none"> Depth gauge <ul style="list-style-type: none"> Left: to check the drilled depth Right: to bend the neck of the EM (MS) provisional type MS narrow narrow ridge type cannot be bent Parallel pin is used to confirm the path of the implant after drilling <ul style="list-style-type: none"> MSPP: lower diameter Ø1.5/upper diameter Ø1.8 MSPPN: lower diameter Ø1.5/upper shape is same as the abutment portion of the MS narrow ridge 	Depth Gauge		HMDTGG	
	Parallel Pin		HMSPP HMSPPN	

Torque Driver Handle	
Description	Image/Item code
<ul style="list-style-type: none"> Used for initial insertion by hand after fastening to torque driver 	 HMSTH

Driver Separator	
Description	Image/Item code
<ul style="list-style-type: none"> If the MS implant is jammed in the Driver, the Driver Separator can be leveraged to separate the two 	 HMSDS


MS Removal Tool		
Description	Image	
<ul style="list-style-type: none"> Easy removal of fractured EM Implant (Narrow Ridge) The tool is used by rotating in the reverse direction after assembling to the universal handle Options based on diameter of fractured implant For Ø 2.0, use orthodontic screw removal tool (code: OSRT20E) <p>※ Disposable. Do not reuse</p>		
D/Ø	Ø2.5	Ø3.0
	HMRT25E	HMRT30E

Drilling Sequence EM (MS) Drill

Narrow Ridge | Denture | Provisional


(Length: 10mm)

Ø1.8mm

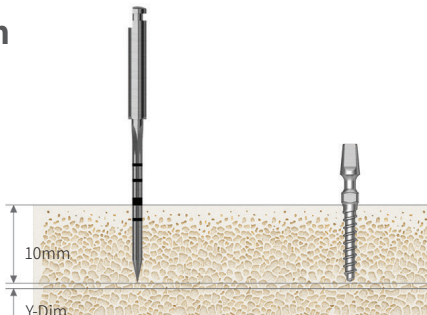


Bone Quality	Lance Drill	Ø1.8 Implant
Soft	▶	Implant Placement
Normal	▶	
Hard	▶	

Ø2.0mm

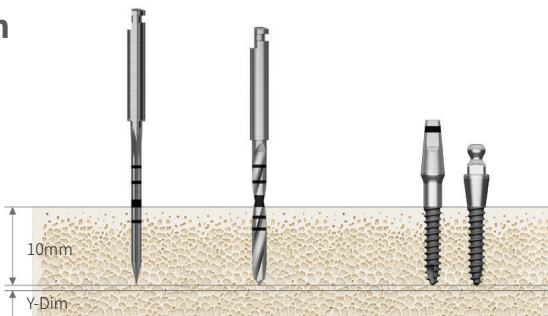


Bone Quality	Lance Drill	Drill (Ø1.8)	Ø2.0 Implant
Soft	▶		Implant Placement
Normal	▶		
Hard	▶	▶	

Ø2.5mm

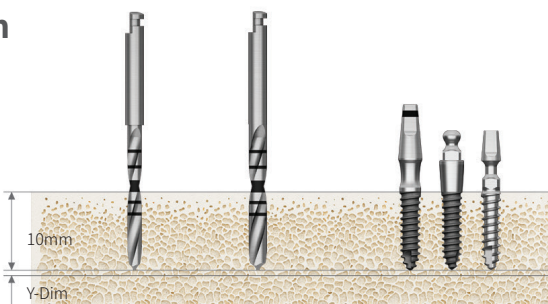



Bone Quality	Drill (Ø1.8)	Drill (Ø2.0)	Ø2.5 Implant
Soft	▶		Implant Placement
Normal	▶		
Hard		▶	

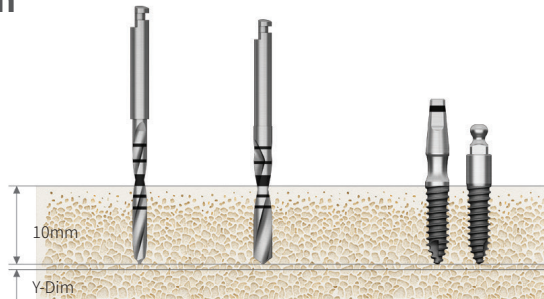

Ø3.0mm





Bone Quality	Drill (Ø1.8)	Drill (Ø2.5)	Ø3.0 Implant
Soft	►		Implant Placement
Normal	►		
Hard		►	



Surgical Instrument Kit


Abutment Positioning Driver				
Description	H + G/H	Length	Item Code	Image
<ul style="list-style-type: none"> Used for assembling the abutment in the prosthetic process after placing an implant ※ For Transfer Abutment only Function to help convenient and stable mounting and tightening of the abutment being pushed away by gingiva Used according to the H and G/H lengths of the abutment to be removed as shown below 	5.0, 6.0, 7.0, 8.0, 9.0	Short (≤ 9)	HAPDS	
	10, 11, 12, 13, 14	Long (≥ 10)	HAPDL	


NoMount Torque Driver for ET				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Directly connects to an ET Implant for placement with a Torque Wrench Ensure correct and complete seating before applying torque; loose connection may cause implant fracture C= Connection 	Mini	Short (19)	HGSNMT32S	
		Long (26.6)	HGSNMT32L	
		Ex. Long (33.6)	HGSNMT32E	
	Regular	Short (19)	HGSNMT35S	
		Long (26.6)	HGSNMT35L	
		Ex. Long (33.6)	HGSNMT35E	


NoMount Torque Driver for SS				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Directly connects to a SS Implant for placement with a Torque Wrench Ensure correct and complete seating before applying torque; loose connection may cause implant fracture *C = Connection 	Regular / Wide	Short (16.8)	HSSNMT39S	
		Long (26.8)	HSSNMT39L	

NoMount Driver for EK				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Ø3.5 implant is combined with the bottom of the lower marking Ø4.0, Ø4.5, Ø5.0, Ø6.0 and Ø7.0 implants are combined with the upper part of the lower marking The distance between the two laser marking is 0.5mm C= Connection 	Regular	Short (27.6)	HKSNMDCRS	   Ø4.0, Ø4.5, Ø5.0, Ø6.0, Ø7.0 Ø3.0, 3.5 Implant Implant
		Long (32.6)	HKSNMDCRL	
		Extra Long (37.6)	HKSNMDCRE	

Implant Driver for ET				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Connects directly to an ET implant for final adjustments to the implant's depth *C = Connection 	Mini	Short (17)	HGSMFDS	
		Long (24)	GSMFDL	
		Ex. Long (34)	HGSMFDE	
	Regular	Short (19)	HGSRFDS	
		Long (26.6)	GSRFDL	
		Ex. Long (33.6)	HGSRFDE	

Implant Driver for SS				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Connects directly to a SS implant for final adjustments to the implant depth *C = Connection 	Regular/ Wide	Short (14)	HSSRFDS	
	Regular/ Wide	Long (24)	SSRFDL	
	Regular/ Wide	Ex. Long (31)	HSSRFDE	

Implant Driver for EK				
Description	C	Length	Item Code	Image
<ul style="list-style-type: none"> Connects directly to an EK implant for final adjustments to the implant's depth *C = Connection 	Regular	Short	HKSFDS	
		Long	HKSFDL	

Torque Extension				
Description			Item Code	Image
<ul style="list-style-type: none"> Extends the length of an instrument by 10mm Connects to the torque wrench 			HOTE	

Surgical Instrument Kit

Simple Mount Driver			
Description	Length	Item Code	Image
<ul style="list-style-type: none"> Connects to mounted implants for placement For use with a handpiece/implant motor 	Short (20.1)	HASMDS	
	Long (26.5)	HASMDL	


Simple Mount Extension			
Description	Length	Item Code	Image
<ul style="list-style-type: none"> Extends the length of the simple mount driver and converts it for use with the Torque Wrench 	Short (14.5)	HASMES	
	Long (20.5)	HASMEL	


Simple Open Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> Disengages the simple mount when bone quality is poor Easy insertion into the mouth with a neck angle of 30° 	SPOW	


Removal Tool for Implant Mount			
Description	Application	Item Code	Image
<ul style="list-style-type: none"> Removes the mount if the mount becomes wedged in the implant Used with Driver Handle or Torque Wrench Removes the mount screw, insert the Removal Tool into the mount, and turn clockwise App = Application 	Mini (ET,US)	HERFM	
	Regular (ET,US) Wide (SS)	HHRFR	
	Wide (US)	HERFW	


Depth Gauge		
Description	Item Code	Image
<ul style="list-style-type: none"> Measures drilling depth (7~15mm) 	ODG	


Positioning Guide			
Description	W/L	Item Code	Image
<ul style="list-style-type: none"> Help set the drilling interval for implant insertion Insert after initial drilling 	2.5 / 21.5	HAPG201	
	6.0 / 17.5	HAPG202	
	11 / 17.5	HAPG203	

Tissue Height Gauge for ET		
Description	Item Code	Image
<ul style="list-style-type: none"> Connects to the ET implant to measure the height of the gingiva in relation to the implant 	HGTSHG	


Ratchet Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> It prevents wrench from backdriving Excessive torquing may cause damage to the bone or the inside of a implant 	CITQW-1185A	

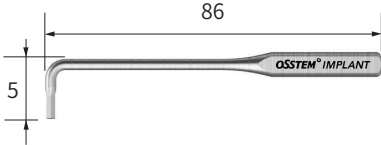
L-Wrench		
Description	Item Code	Image
<ul style="list-style-type: none"> 1.2 hex driver for hard to reach areas like narrow intermaxillary areas Torque indication: when the wrench starts to bend (around 10°), it is possible to apply 5~8Ncm of torque 	HLWC	


Torque Wrench - Bar Type		
Description	Item Code	Image
<ul style="list-style-type: none"> Adjusts the implant depth, and tightens abutments, screws, etc. Pull the bar back until the desired torque value is reached 	TQWCB	


Torque Wrench - Spring Type		
Description	Item Code	Image
<ul style="list-style-type: none"> Applies a precise amount of torque (10/20/30Ncm) to the screw and abutment The neck of the torque wrench will bend when the exact amount of torque has been delivered Do not continue to torque after the neck has bent; excessive force may cause screw fracture etc. 	HTW30	


Surgical Instrument Kit

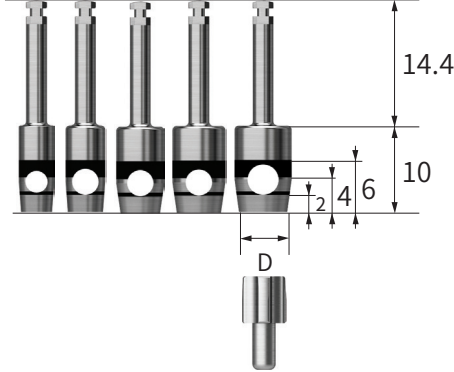Tissue Punch					
Description/Item code				Image/Guide	
<ul style="list-style-type: none"> For flapless surgery Laser marking to measure the height of gingiva, marked in 2mm increments Packing unit: tissue punch + guide pin Recommend to use a tissue punch smaller than the healing abutment by 0.7 to 1.5mm 					
ET	SS	D/Ø	Item Code		
Ø 4.0/4.5	-	Ø3.3	HSTP33		
Ø 4.5/5.0	Ø 4.8	Ø3.8	HSTP38		
Ø 5.0	-	Ø4.3	HSTP43		
Ø 6.0	Ø 6.0	Ø4.8	HSTP48		
Ø 6.0	Ø 6.0	Ø5.3	HSTP53		
Application healing abutment standard					


Bone Profiler					
Description/Item code				Image/Guide	
<ul style="list-style-type: none"> Used to remove bone around the implant after first or second stage surgery Connect the Guide Screw to the implant in order to center the profiler Guide screw protects the implant's platform from damage Packing unit: bone profiler + guide screw *C = Connection 					
Guide Screw	D (Healing Abutment)	ET Mini / Regular	EK Regular		
ET (Mini + Regular)	Ø4.0	HGSBP40	HKSBP40		
EK (3.0/3.5 + Regular)	Ø4.5	HGSBP45	HKSBP45		
Regular	Ø5.0	HGSBP50	HKSBP50		
	Ø6.0	HGSBP60	HKSBP60		
	Ø7.0	HGSBP70	HKSBP70		

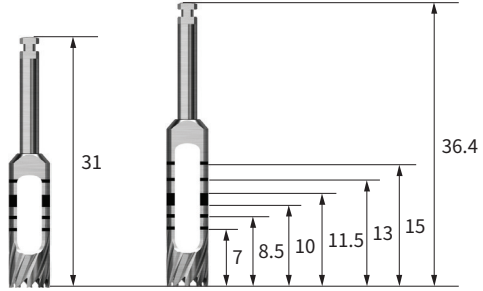
Trephine Drill			Image/Guide	
Description/Item code			Image/Guide	
<ul style="list-style-type: none"> Harvests bone or removes a failed implant Used to remove septal bone Can also be used as the initial drill for ultra-wide implants 				
D/Ø (Inner/Outer)	Short	Long		
3.7/4.5	HTD37S	HTD37		
4.2/5.0	HTD42S	HTD42		
4.7/5.5	HTD47S	HTD47		
5.2/6.0	HTD52S	HTD52		
5.7/6.5	HTD57S	HTD57		
6.2/7.0	HTD62S	HTD62		

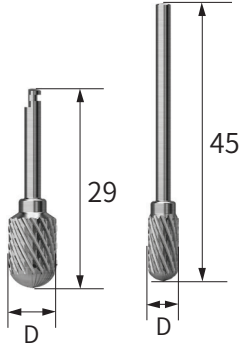
Crest Remover			Image/Guide	
Description/Item code			Image/Guide	
<ul style="list-style-type: none"> Marking the implant placement position after removing the narrow alveolar ridge horizontally Recommended drilling speed <ul style="list-style-type: none"> - Angled type: 1,200~1,500rpm - Straight type: 15,000~30,000rpm 				
L	29	45		
D Ø5.0 D Ø7.0	CERM50A -	CERM50S CERM70A		

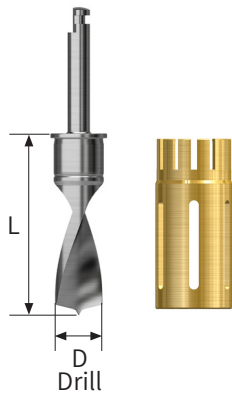
AutoBone Collector®			Image/Guide	
Description/Item code			Image/Guide	
<ul style="list-style-type: none"> Used for autogenous bone collecting Comes in a Drill + Stopper set Recommended drilling speed: 300~600rpm Number of uses for the drill and stopper: 50 times <p>※ Before initial drilling, connect the stopper to the first stage locking and harvest autogenous bone while drilling 4mm into the second stage locking (after harvesting, stop the drill and remove as it is with autogenous bone kept in the stopper)</p>				
D	Short (18.94)	Long (21.94)		
Ø3.0	ABC304S	ABC304L		
Ø4.0	ABC404S	ABC404L		
Ø5.0	ABC504S	ABC504L		
Ø6.0	ABC604S	ABC604L		

Surgical Instrument Kit

Machine Driver Handle		
Description	Item Code	Image/Guide
<ul style="list-style-type: none"> Tool used convert engine type surgical tools into a manual type 	HMDH	

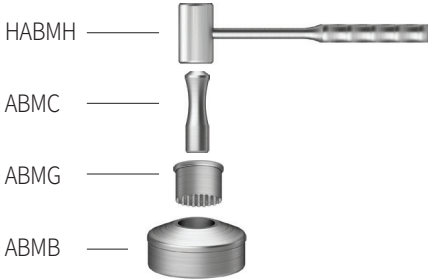Bone Mill		
Description	Item Code	Image
<ul style="list-style-type: none"> Grinds harvested autogenous bone 	HABM	<div> <div>HABMH</div> <div>ABMC</div> <div>ABMG</div> <div>ABMB</div>  </div>

Anterior Hand Driver for Implant		
Description	Item Code	Image
<ul style="list-style-type: none"> Manually torque implants in the anterior area Connect to a NoMount torque driver or a implant driver Excessive torque may cause damage to the implant and/or driver 	HAHDI	

Torque Handle		
Description	Item Code	Image
<ul style="list-style-type: none"> Connectable to a contra-angle handpiece (Hand-Piece gear ratio to 1:1) Used to connect healing abutments, cover screws, abutment screws, orthodontic screws, etc. (Note: after connecting, make sure that it is tightened with a torque wrench) Excessive torque may cause damage to the screw and/or hand piece 	HTQHD	



the 1990s, the number of people in the world who are under 15 years of age has increased from 1.1 billion to 1.5 billion, and the number of people aged 65 and over has increased from 0.5 billion to 0.7 billion (United Nations 2002).

There are a number of reasons why the world population is ageing. One of the main reasons is that the number of people who are surviving to old age has increased. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality.

Another reason why the world population is ageing is that the number of people who are having children is decreasing. This is due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.

The world population is ageing, and this is a trend that is likely to continue. This is due to a number of factors, including improvements in healthcare, better nutrition, and a decline in infant mortality. It is also due to a number of factors, including a decline in fertility rates, a decline in the number of people who are having children, and a decline in the number of people who are having children at a young age.



Smiles that last a life time

Hiossen Implant Inc.

270 Sylvan Ave. Ste 1130, Englewood Cliffs, NJ 07632
www.hiossen.com Email: marketing@hiossen.com

📷 @hiossen_implants 📘 @HiossenImplants 🌐 @Hiossen

